TELEQUIPMENT

SUPPLIED BY
Cooke International
TEL (+44)(0) 1243 555590
Web: http://www.cooke-int.com

OSCILLOSCOPE
TYPE D32

703631

INSTRUCTION MANUAL

TELEQUIPMENT ®

DANGER

It is not possible to screen all high voltages, so care should be taken not to touch high voltage tags. Also where possible the instrument should be unplugged AND switched off during servicing. A BLEEDER PATH FOR THE EHT IS NOT PROVIDED, so after switching off and before touching any internal parts, the EHT should be discharged by temporarily shorting the appropriate points to chassis, (for instance the CRT cathode pin and PDA connector where applicable).

FOR SERVICING AND SPARES ENQUIRIES
SEE THE INFORMATION AT START OF SECTION 5.

TELEQUIPMENT is a registered trade mark of TEKTRONIX U.K. LTD.

TEKTRONIX U.K. LTD
313 Chase Road,
Southgate,
London N14 6JJ
ENGLAND.

Telephone:
01-882 6100
Telex: 262004
Cables:
TELEQUIPT LONDON N14

TEKTRONIX INC.,
P.O. Box 500,
Beaverton,
Oregon (97005),
U.S.A.

Telephone:
(503) 644-0161
Telex: 36 0485
Cables:
TEKTRONIX

OSCILLOSCOPE
TYPE D32

703631

INSTRUCTION MANUAL

Issue 8 (703301)
November 1977
©Copyright (1975) by
TEKTRONIX U.K. LTD.

070-1797-00

Printed in England by D & H NEWMAN LTD, 29 Harcourt Street, London W1. 01-262 6356

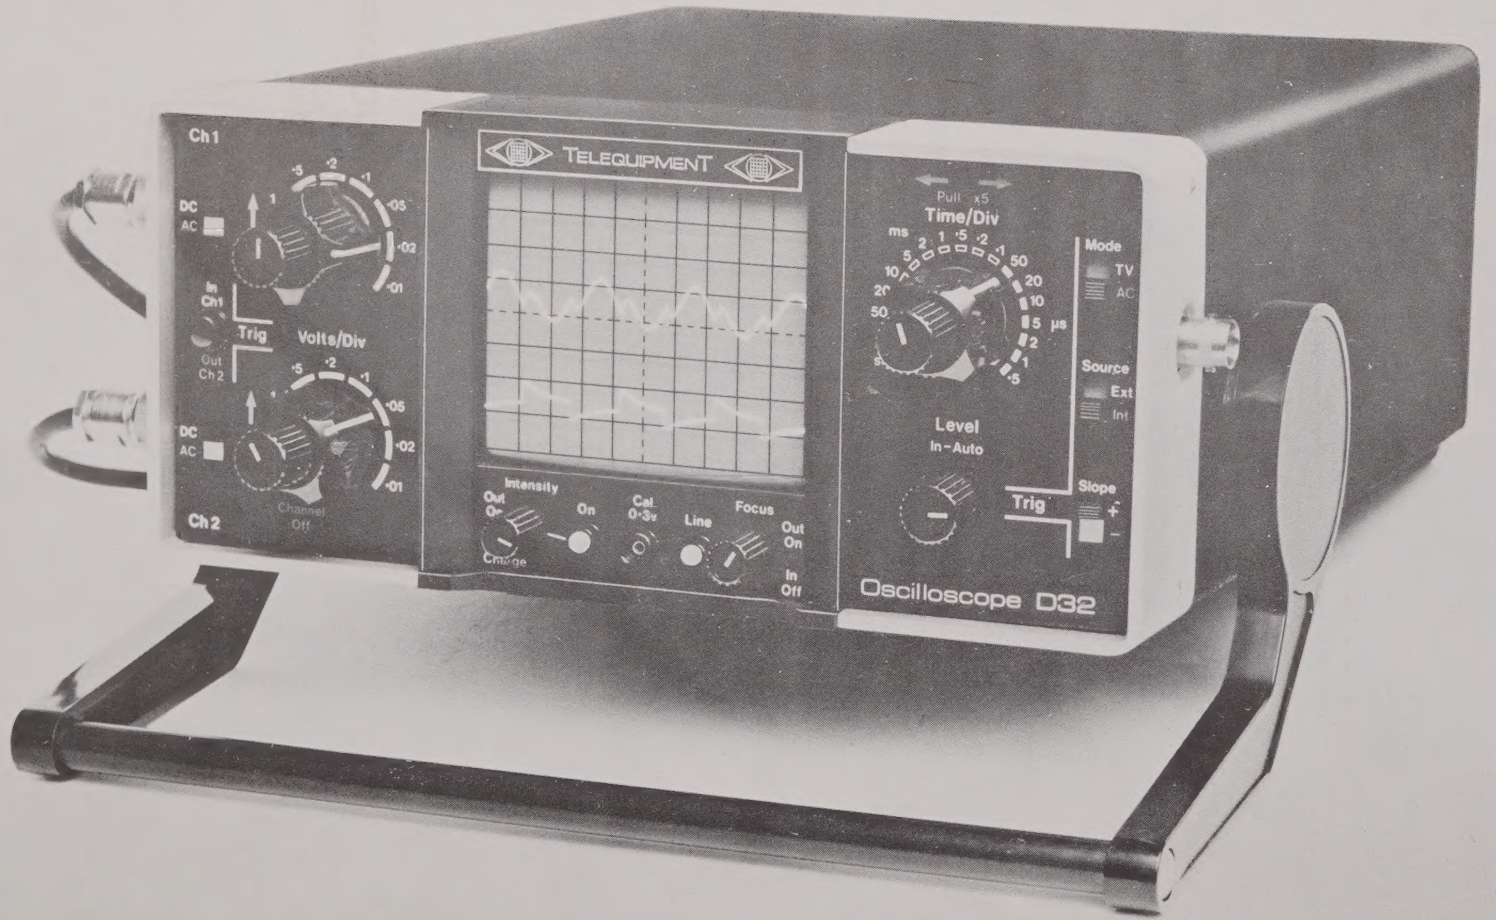
Ch1
DC
AC
In
Ch1
Trig
Out
Ch2
Volts/Div
DC
AC
Channel
Off
Ch2
TELEQUIPMENT
Intensity
Out
On
Charge
On
Cal
0·3v
Line
Focus
Out
On
In
Off
Pull x5
Time/Div
ms
μs
Level
In-Auto
Trig
Mode
TV
AC
Source
Ext
Int
Slope
+
–
Oscilloscope D32

TELEQUIPMENT TYPE D32
OPERATING INSTRUCTIONS

To obtain a trace quickly and easily we suggest you try the following procedure.

1. Put all slide switches down (↓).
2. Push in (TRIG selector (CH1)
   (LEVEL control (to auto)
   (↔ Horizontal position.
3. Switch on by pulling (or rotating) the INTENSITY control. (If connected to an AC line pull FOCUS control out).

D32 – Betjeningsanvisning

For å hjelpe Dem med førstegangsbruk av dette oscilloskop, anbefaler vi følgende fremgangsmate:

1. Still alle glidevendere (slide switches) i nederste stilling – (↓)
2. Trykk inn (Trig selector
   (level control
   (Horizontal position
3. Slå på oscilloskopet ved å dra ut (eller vri på) Intensity control. (Hvis oscilloskopet er koplet til lysnettet, trekker De ut Focus controlknappen).

BEDIENINGSVOORSCHRIFT TELEQUIPMENT D32

De onderstaande procedure wordt geadviseerd bij het in gebruik nemen van deze oscilloscoop.

1– Plaats alle schuifschakelaars in de onderste stand (↓).

2– Druk de volgende schakelaars in:
- Triggerkeuzeschakelaar ("trig", links op het frontpaneel).
- Niveauregeling ("level", rechts op het frontpaneel).
- Horizontale positie (buitenste knop van de Time/Div. knop rechts op het frontpaneel).

3– Schakel het instrument in door de intensiteitsknop uit te trekken. (Bij voeding uit het lichtnet tevens de focusregelingsknop uitrekken).

PLAQUETTE TELEQUIPMENT – MISE EN SERVICE D 32 – CONSEILS DE MISE EN SERVICE

Afin de faciliter la mise en service de cet oscilloscope, nous vous recommandons de procéder comme suit:

1. Pousser tous les commutateurs à glissière vers le bas (↓).
2. Enclencher les boutons 'Trig Selector', 'Level Control', 'Horizontal Position'.
3. Mettre en route en tirant (ou tournant) le bouton 'Intensity Control' (fonctionnement sur réseau : mise en service en tirant le bouton 'Focus').
4. Tourner la commande 'Intensity' à fond vers la droite (intensité maximale).

BEDIENUNGSKARTE D32

Diese Bedienungskarte soll bei der ersten Inbetriebnahme eine kleine "Hilfestellung" geben. Beachten Sie bitte die folgenden Punkte:

1. Setzen Sie alle Kippschalter nach unten.
2. Drücken Sie die Bedienungselemente TRIG CH1, LEVEL, HORIZ POSITION.
3. Schalten Sie das Gerät ein, indem Sie den Drehknopf INTENSITY aus seiner Rasterstellung nach rechts bewegen (bei Netzbetrieb FOCUS ausschalten).
4. Wählen Sie die höchste Helligkeit (INTENSITY auf Rechtsanschlag).

ISTRUZIONI OPERATIVE DEL MODELLO D32

Al fine di aiutarVi nel primo modo di impiego di questo oscilloscopio, suggeriamo di seguire la seguente procedura:

1– Porre tutti i commutatori a levetta in basso (↓).

2– Premere i comandi
- selettore di sincronismo
- comando di livello
- posizione orizzontale

3– Accendere lo strumento tirando (o ruotando) il comando Luminosità. (Se lo strumento è collegato alla rete, tirare anche il comando FUOCO).

4– Ruotare il comando Luminosità tutto in senso orario.

D32 HANDLEDNING

För att hjälpa Er när Ni första gången ska använda Ert oscilloscope föreslår vi att Ni följer nedanstående punkter.

1. Stall samtiga switchar i läge ner.
2. Tryck in knapparna TRIG, LEVEL och PULL x 5.
3. Slå på oscilloscopet genom att vrida ratten INTENSITY medurs. (Om oscilloscopet är anslutet till nätet, drag även ut ratten FOCUS).
4. Vrid ratten INTENSITY max medurs.

D 32
START INSTRUKTION

For at lette forståelsen og første start af instrumentet, anbefaler vi nedenstaende procedure:

1. Skub alle skydeomskiftere i deres nederste position.
2. Kontroller, at trig-selector, trig-level kontrol og horizontal position er indtrykket.
3. Tænd instrumentet ved at dreje (eller trække) intensitetskontrollen. (Hvis instrumentet er tilsluttet lysnettet, træk også focuskontrollen ud).

INSTRUCCIONES DE FUNCIONAMIENTO DEL OSCILOSCOPIO D32

Con el objeto de ayudarle a una fácil puesta en marcha de éste osciloscopio, nosotros le sugerimos el siguiente proceder:

1– Ponga todos los interruptores hacia abajo (↓).

2– Introduzca a la posición interior los botones "Trig Selector" "Level Control" y "Horizontal Position".

3– Commute "on" sacando o girando el control de intensidad "Intensity" (Si está conectado a tensión de red saque hacia fuera el botón control del Foco "Focus").

INSTRUÇÕES DE OPERAÇÃO DO D32

Procedimentos recomendados para a primeira operação deste osciloscôpio:

1– Coloque todos os comutadores de accionamento vertical na posição mais baixa (↓).

2– Carregue (Selector de "trigger"
(no control de nível
(na posição horizontal (↔)

3– Ligue a alimentação puxando (ou rodando) o controle de intensidade (se estiver ligago à alimentação AC puxe também o controle de focagem).

4. Skru Intensity til maksimum (til høyre).
5. Skru Vertical og Horizontal posisjonskontroller slik at orange-merker blir vertikale.
6. Juster Intensity og Focus-kontrollene slik at De får en fokusert stråle med passende intensitet.
7. Juster Trace Rotate (på instrumentets bakside) slik at strålen blir horisontal.
8. Kople til et signal til CH1-inngangen og velg en passende følsomhet Volts/div og tidsbase Time/div, slik at De får en kurve som står stille og som har passende høyde og bredde.

4. Turn INTENSITY to maximum (fully clockwise).
5. Turn ↕ (vertical) and ↔ (Horizontal) position controls so that the orange marks are vertical.
6. Adjust INTENSITY and FOCUS controls for a focussed line(s) of suitable intensity.
7. Adjust TRACE ROTATE (situated on the rear panel) for horizontal line(s).
8. Connect an input signal to CH1 INPUT and select the appropriate VOLTS/DIV and TIME/DIV positions to give a locked trace of convenient signal amplitude and width.

5. Placer les réglages de position (↕) à mi-course (repères orange verticaux).
6. Régler les commandes d'intensité (Intensity) et de focalisation (Focus) pour obtenir une représentation satisfaisante.
7. Régler l'alignement horizontal de la trace à l'aide de la commande 'Trace Rotate' (à l'arrière de l'appareil).
8. Connecter un signal à l'entrée Voie 1 (CH 1) et choisir le facteur de déflexion (Volts/Div) et la vitesse de balayage (Time/Div) permettant d'obtenir une représentation stable, d'amplitude et de largeur satisfaisantes.

4– Draai de intensiteitsregeling op maximaal (volledig naar rechts).
5– Draai de verticale en horizontale regelingen (buitenste knop van Volts/Div. en Time/Div. knoppen) totdat de oranje markeringstreepjes in verticale stand zijn.
6– Draai de intensiteits– en focusknoppen totdat een gefocusseerde lijn(en) van voldoende intensiteit verkregen is.
7– Indien noodzakelijk, de lijn(en) horizontaal afregelen met draaischakelaar ("Trace Tilt Correction") op het achterpaneel.
8– Sluit nu een signaal aan op kanaal 1 (ch 1) en kies de meest geschikte Volts/Div. en Time/Div. standen voor een golfvorm van bruikbare amplitude en breedte.

5– Ruotare i comandi di posizione verticale ed orizzontale in modo che i riferimenti arancione sui comandi stessi siano a metà corsa.
6– Regolare i comandi di Luminosità e Fuoco per ottenere sullo schermo un tracciato di luminosità e fuoco desiderati.
7– Regolare il comando rotazione traccia (situato sul pannello posteriore) per un corretto allineamento della stessa con il reticolo.
8– Applicare un segnale all'ingresso del canale CH 1 e, agendo sui comandi Volt/DIV e Tempo/DIV, ottenere sullo schermo un tracciato stabile di ampiezza e durata desiderati.

5. Stellen Sie die vertikalen und horizontalen Positionseinsteller so ein, dass die orangefarbigen Markierungsstriche senkrecht stehen.
6. Stellen Sie mit Hilfe der Bedienungselemente INTENSITY und FOCUS einen gut fokussierten Ablenkstrahl mit ausreichender Helligkeit ein.
7. Benutzen Sie, falls notwendig, das Justierelement TRACE ROTATE (Rückwand) dazu, die Strahlspur parallel zu den horizontalen Rasterlinien auszurichten.
8. Schliessen Sie ein Signal an den Eingang CH1 INPUT und wahlen Sie mit Hilfe der Stufenschalter VOLTS/DIV und TIME/DIV den entsprechenden Spannungs- und Zeitbereich.

4. Drej intensiteten helt op (med uret).
5. Drej de tre positionsknapper, så de orange mærker står lodret.
6. Juster intensitet og focus til skarpest stråle og med rimeligt lys.
7. Juster eventuelt trace rotate (placeret på bagsiden) så strålerne følger linierne.
8. Tilslut så signal på kanal 1 og drej på volts/div. til passende signalstørrelse og på time/div. til passende bredde på signalet.

5. Vrid rattarna för vertikala och horisontala positionerna, så att den orange markeringen är lodrät (från centrum och uppåt).
6. Justera ljusstyrkan och skärpan i strålarna med rattarna INTENSITY och FOCUS till lämpligt värde.
7. Justera med ratten TRACE TILT som finns på baksidan av oscilloscopet så att strålarna blir parallella med rutnätet.
8. Anslut signalen som ska mätas till ingången CH1 och ställ in storleken på signalen med omkopplaren VOLTS/DIV samt sveptiden med omkopplaren TIME/DIV.

4– Rode o controle de intensidade para o máximo (no sentido dos ponteiros do relógio).
5– Rode os controles de posição vertical e horizontal de forma a que as marcas laranja fiquem verticais.
6– Ajuste os controles de Intensidade e Focagem de forma a obter uma linha focada e com intensidade desejada.
7– Ajuste o controle de relação de traco de forma a obter uma linha horizontal. (Situado no painel traseiro).
8– Ligue um sinal à entrada CH1 e seleccione os comutadores volt / div e Time/div de forma a representar o sinal com as amplitudes e largura convenientes.

4– Gire la intensidad "Intensity" al máximo (todo hacia las agujas del reloj).
5– Gire las posiciones verticales y horizontales para que la raya naranja esté en posición vertical.
6– Ajuste la intensidad y el control de foco para que aparezca un trazo bien definido y suficientemente claro.
7– Ajuste la rotación de trazo "Trace Rotation" para una suficiente coincidencia con la horizontalidad de la gratícula.
8– Conecte una cierta señal en la entrada del canal CH1 y seleccione las apropiadas escalas de Volts/div y Time/div para conseguir una visualización adecuada de tal señal.

INTRODUCTION

The D32 is a 10MHz, all solid state, dual trace portable oscilloscope. It can operate from internal batteries or an external AC supply and incorporates a built-in battery charger.

The dual trace vertical system displays either channel separately; alternates between channels and chops between channels at approximately 100kHz rate. The use of FET input circuitry ensures minimum drift and fast stabilization time.

The design of this instrument is subject to continual development and improvement, therefore minor changes in detail from the information contained herein may be incorporated. These changes which usually affect the Component Lists and Circuit Diagrams are described on Amendment Lists issued at regular intervals between reprints.

Any Amendment List appertaining to this manual is located in the pocket inside the back cover.

Throughout this manual all references to the front panel controls are in full and in capital letters, e.g. INTENSITY.

WARNING

To all users of this manual:

1. The instrument is switched off by pushing in the INTENSITY control.

2. The battery charger is switched off by pushing in the FOCUS control.

3. The instrument should have batteries fitted at all times because in addition to being a DC supply source they act as high value capacitors when operating on an AC supply.

4. Before fault finding or servicing is carried out on this instrument, careful attention should be paid to the warning at the start of Section 4.

If this instrument is returned for servicing the owner is requested not to send the Probe or Plug Assemblies unless they are suspect. This is to facilitate packing and lessen the risk of damage during transit.

CONTENTS

SECTION — Page

1 SPECIFICATION
- Accessories available (extras) ... 1/2
- Accessories (standard) ... 1/2
- Cal Output Socket ... 1/2
- Cathode Ray Tube (CRT) ... 1/1
- General
  - Cooling ... 1/2
  - Power Requirements ... 1/2
  - Size ... 1/2
  - Temperature Range, ambient ... 1/2
  - Weight ... 1/2
- Horizontal Deflection
  - Sweep Rates ... 1/1
  - Trigger ... 1/1
- Vertical Amplifiers
  - Bandwidth ... 1/1
  - Display Mode ... 1/1
  - Vertical Deflection ... 1/1

2 OPERATING INSTRUCTIONS
- Additional Facilities — Use of
  - Trigger Source ... 2/3
  - Slope ... 2/3
  - Mode ... 2/3
  - Level ... 2/3
- Basic Applications
  - Frequency Measurements ... 2/3
  - Peak to Peak Voltage Measurement ... 2/3
- Battery Operation
  - Batteries ... 2/1
  - Battery Charging ... 2/1
- First Time Operation
  - Setting the controls ... 2/2
  - Switch On ... 2/2
- Input and Output Sockets ... 2/2
- Mains Operation ... 2/1
  - Table of voltage selector settings ... 2/1
- Operation of Controls
  - CRT ... 2/1
  - Horizontal ... 2/1
  - Trig (pick off) ... 2/1
  - Vertical ... 2/1
- Pre Operational Check ... 2/1

3 CIRCUIT DESCRIPTION
- Attenuator ... 3/1
- Battery Charger ... 3/2
- Bright Line Auto ... 3/1
- Calibrator ... 3/2
- Cathode Ray Tube ... 3/2
- Convertor Power Supply Unit ... 3/2
- Horizontal Amplifier ... 3/2
- Timebase ... 3/1
- Trigger ... 3/1
- Unblanking ... 3/1
- Vertical Output Amplifier ... 3/1
- Y Amplifier (CH1 and CH2) ... 3/1

SECTION — Page

4 MAINTENANCE AND CALIBRATION
- Calibration Procedure
  - Astigmatism and Geometry ... 4/3
  - Balance — CH1 and CH2 ... 4/3
  - Battery Charge Rate and Initial Setting ... 4/3
  - Gain and Attenuator — CH1 and CH2 ... 4/3
  - HF Response — CH1 and CH2 ... 4/4
  - Internal Calibrator ... 4/4
  - Sweep Accuracy ... 4/4
  - Sweep Stability and Length ... 4/4
  - Supply Line Voltages ... 4/3
  - Table of Expected Voltages ... 4/3
  - Trigger Sensitivity ... 4/4
  - TV Trigger ... 4/4
- Introduction ... 4/1
- Mechanical
  - Access to Interior ... 4/1
  - CRT Fitting ... 4/1
  - CRT Removal ... 4/1
  - Replacing R/H or L/H Front Panel ... 4/1

5 COMPONENTS LIST
- Assemblies
  - Centre Assembly and Rear Panel ... 5/9
  - L/H Side Sub-Assembly ... 5/9
  - Lower Sub-Assembly ... 5/9
  - R/H Side Sub-Assembly ... 5/9
- Electrical Components ... 5/2
- Mechanical Parts ... 5/10
- Table of Circuit References ... 5/1

6 CIRCUIT DIAGRAMS — Figure
- Channel 1 Input Stage ... 1
- Channel 2 Input Stage ... 2
- Y Output and Chop — Alternate Bistable ... 3
- Trigger Circuit ... 4
- Sweep Generator, Unblanking and X Amp ... 5
- Calibrator and CRT ... 6
- Battery Charger and Power Supply ... 7
- Time/Div Switch ... 8

Table showing the Printed Circuit boards in which each circuit is located ... Page 6/1

SECTION 1
SPECIFICATIONS

1.1 CATHODE RAY TUBE (CRT)

	Rectangular flat faced CRT with mesh screen.
Display area	10 x 8 divisions (each division = 0.7 cm.)
Phosphor	P31
Overall accelerating Potential	3 kV

1.2 VERTICAL AMPLIFIERS

1.2.1 DISPLAY MODE

CH1
CH1 and CH2 alternate
CH1 and CH2 chopped (at 100 kHz)
Chop or alternate selected automatically on TIME/DIV switch

1.2.2 BANDWIDTH (3db)

DC	DC – 10 MHz
AC	3 Hz – 10 MHz

1.2.3 VERTICAL DEFLECTION

Calibrated (9 ranges 1.2.5 Sequence)	10 mV/div – 5 V div ± 5%
Input impedance	1 MΩ in parallel with 32 pF.
Max. Input voltage	± 250 V peak

1.3 HORIZONTAL DEFLECTION

1.3.1 SWEEP RATES (19 ranges in 1, 2, 5 sequence)

X1	500 ms/div – 0.5 μs div ± 5%
X5	100 ms/div – 200 ns/div ± 7% 200 ns/div – 100 ns/div ± 10%

1.3.2 TRIGGER

Level	Fully variable over 8 divisions on all waveforms.
Auto	Bright line in absence of trigger signal, automatic trigger on symetrical waveforms over 1 div. with restricted level control.
Mode	AC or TV field for sweep ranges 0.5 sec/div. to 0.1 ms/div. and TV line from 50 μs/div. to 0.5 μs/div.
Source	CH1, CH2 or external. All positive or negative.
Sensitivity	
Internal	
40 Hz – 2 MHz	0.4 div. Level and Auto Trigger
2 MHz – 10 MHz	1 div. Level Trigger
External	
40 Hz – 5 MHz	500 mV approx.
5 MHz – 10 MHz	1 V approx.

1.4 CAL OUTPUT SOCKET

Output Voltage	300 mV ± 1%
Output Impedance	600Ω
Wave Shape	Vertical edge at screen centre — positive with respect to earth.

1.5 GENERAL

1.5.1 POWER REQUIREMENTS

Internal rechargable battery	
Voltage	6 x 1.25 V ('D' CELLS)
Battery life	4 hours approximately continuous use. Built in charger allows the batteries to be charged in 14 hours with the instrument switched off or trickle charges the batteries if the instrument is switched on.
Mains	
Voltage	100–112 V 112–125 V 200–224 V 225–250 V
Frequency	50–400 Hz
Consumption	14 VA

1.5.2 SIZE

Height (stand retracted)	105 mm
Width	230 mm
Depth	288 mm

1.5.3 WEIGHT

4.5 kg

1.5.4 COOLING

Convection

1.5.5 TEMPERATURE RANGE (AMBIENT)

Operational	0° to 35°C
Storage	−10°C to 40°C

1.6 STANDARD ACCESSORIES SUPPLIED WITH THE INSTRUMENT

ACCESSORY	QUANTITY	PART NUMBER
Cover front protection	1	437-0171-01
Manual	1	070-1797-00

1.7 ACCESSORIES AVAILABLE AS EXTRAS

ACCESSORY	PART NUMBER (for ordering)
Carrying case	016-0601-00
Carrying case (attaché style)	016-0374-00
Calibration lead	012-0571-00
Probe type TP2 (X10 attenuator)	
4.5 foot cable	010-0270-00
6.0 foot cable	010-0270-02
BNC connector plugs	131 0649
Allen key 1.5mm A/F	
External battery adaptor	119-0766-00

SECTION 2
OPERATING INSTRUCTIONS

2.1 PRE-OPERATIONAL CHECK

Although this instrument is robust and is subjected to stringent checks before leaving our factory, it should be checked externally for possible damage. In the case of damage contact the carriers and your local Tektronix field office immediately.

Before switching the instrument on it is recommended that this chapter is read right through and that some time be spent in becoming familiar with the controls.

Remove the front protection cover by uncoupling the retainers from the BNC sockets and gently pulling the cover off.

2.2 BATTERY OPERATION

2.2.1 BATTERIES

The batteries fitted in this instrument have been charged before despatch. If a considerable time has elapsed between dispatch and putting the batteries into use, a self discharge process, may result in the batteries either being discharged or in a low state of charge. A battery test socket in provided on the rear panel to allow a check to be made. Using a voltmeter of 20 kΩ/Volt connected between the + and — of the rear battery check socket a reading of 6.8 volts to 9 volts should be obtained. If no voltage reading at all is obtained the DC fuse should be checked. If the voltage is low the batteries should be charged as follows.

2.2.2 BATTERY CHARGING

Before carrying out the charge procedure the mains cable should be fitted and the voltage selector switches set to the available mains voltage. For this procedure see the paragraph headed Mains Operation. Having carried out this procedure the unit should be plugged into the mains supply. The LINE indicator on the front panel should light. The instrument should be OFF. This can be checked by seeing that the switch on the INTENSITY control is pushed in and that the ON indicator is not illuminated. After 14 hours the batteries should be fully charged.

2.3 MAINS OPERATION

The mains cable should be plugged into the back of the instrument and secured using the screws and nuts supplied. Where a standard mains lead is supplied it will be necessary to fit a plug to suit the available supply. The mains cable connections are as follows.

Brown ..... Line
Blue ..... Neutral
Green/Yellow..... Earth

FOR SAFETY REASONS THE EARTH WIRE MUST BE CONNECTED, AND IF AN EXTENSION LEAD IS USED — ADEQUATE EARTH CONTINUITY MUST BE PROVIDED.

Two voltage selector switches are provided. The range switch is located on the under side of the instrument and a tapping switch is on the rear panel. These switches should be set to the available mains supply according to the table below. If the selector switches have to be moved it may be necessary to change the instrument fuse using the alternative one provided. The correct fuse to be fitted is shown in the table. The fuse is located inside the instrument so it is necessary to remove the case as per paragraph 4.2.1. The fuse is the vertically mounted one towards the rear of the instrument.

A.C. LINE VOLTS	RANGE VOLTS	TAPPING	INSTRUMENT FUSE
100—112	112	LO	500 mA
113—125	112	HI	500 mA
200—224	225	LO	250 mA
225—250	225	HI	250 mA

Having carefully checked the fuse rating and voltage selector switch positions the instrument can be plugged into the mains supply. On plugging in, the line indicator should light immediately the FOCUS control is pulled out. With the instrument switched off, the battery charger provides a full charge to the batteries but when the instrument is switched on the charge becomes a trickle charge, to keep the battery voltage topped up

2.4 OPERATION OF CONTROLS

2.4.1 CRT

INTENSITY — varies the display intensity. An instrument ON/OFF switch is fitted to this control.

FOCUS — controls the display definition; a power ON/OFF switch is fitted on this control.

TRACE ROTATION — This control is fitted on the back of the instrument. It allows the trace to be aligned with the horizontal graticule lines.

2.4.2 VERTICAL

VOLTS/ DIVISION — provides attenuation of the input signal in 9 calibrated steps.

Y POSITION ↕ — marked with a double headed vertical arrow. Moves the respective trace in the Y or vertical axis. CH2 POSITION control also has fitted a channel off control which operates when the control is turned fully anti-clockwise position (clicks off).

AC/DC — This selects the input coupling. In the AC position a capacitor is in series with the input, whilst in the DC position the signal is coupled directly to the attenuator.

2.4.3 TRIG (Pick off)

The push button selects the channel required to give a triggering pulse.

2.4.4 HORIZONTAL

TIME/DIV — selects the sweep speed having 19 calibrated steps in the range 500 ms/division to 0.5 μs/division.

X5 — When the X5 switch is pulled out the sweep speeds are magnified by a factor of 5 and therefore the sweep range becomes 100 ms/division to 100 ns/division.

X POSITION ⟷	The X POSITION control uses the same knob as the speed magnifier. When it is rotated it moves the trace in an X or horizontal axis.
TRIG. MODE	Triggering is normally AC coupled (AC position) but when TV is selected, triggering is from a TV frame at sweep speeds of 0.5 s/division to 0.1 ms/division and from a TV line at sweep speeds of 50 μs/division to 0.5 μs/division.
TRIG. SOURCE	In the INT position triggering is from the input signal whilst the EXT position allows triggering from an external source connected to the EXT TRIG. socket.
TRIG. SLOPE	This switch allows triggering on a positive or negative slope of an input waveform.
TRIG. LEVEL	The level control selects the voltage level of the input waveform at which the sweep starts. With the knob pushed in, the AUTO position is selected. In the absence of an adequate trigger signal the sweep generator free runs providing a stable reference trace.

2.5 INPUT AND OUTPUT SOCKETS

CH1, CH2 } INPUT	These sockets connect the input signal to the respective vertical amplifiers.
EXT TRIG.	This socket connects an external signal to the trigger circuit and is used in connection with the trig SOURCE switch.
CAL.	A waveform of 0.3 V amplitude is provided at this socket to allow for the checking of the calibration of the vertical channels. The CAL. waveform can be used to set up a probe, connected to CH1 or CH2 INPUT. With the appropriate VOLTS/DIV switch set to 0.01 V and TIME/DIV switch set to 1 ms/DIV the probe tip should be connected to the CAL. socket. The probe trimmer should be adjusted for the best obtainable square corner. TRIG SOURCE should be set to EXT.
BATT CHECK AND EXTERNAL SUPPLY FACILITY (5 Pin DIN)	This socket is provided to enable the state of charge of the internal batteries to be determined, and to provide a facility for operation from an external supply of 11V DC via an external battery adaptor, available as an accessory.

2.6 FIRST TIME OPERATION

2.6.1 SETTING THE CONTROLS

Set the front panel controls as follows:-

INTENSITY	Fully anti-clockwise — and pushed in.
FOCUS	Central — In.
CH1, CH2 } VOLTS/DIV	0.05 V
CH1, CH2 } AC/DC	DC
CH1 Y POSITION	Central
CH2 Y POSITION	Fully anti-clockwise (should click off)
TRIG. BUTTON	In
TIME/DIV	50 μs
X POSITION	In and central
LEVEL	In and central
MODE	AC
SOURCE	EXT.
SLOPE	+

Connect the CAL 0.3 V socket (2mm) to Input socket. For this operation a lead of 75Ω CO-AXIAL cable is required with a BNC plug at one end and a 2 mm plug at the other. It should be possible to construct such a lead using one of the BNC plugs provided and using locally obtained, coax and a 2 mm plug but in case of difficulty contact your local Textronix field office.

2.6.2 SWITCH ON

1. Switch on by pulling out the FOCUS control and the INTENSITY control.
2. Allow a short while for a trace to appear.
3. Centralize the trace using the X and Y (CH1) POSITION controls.
4. Adjust the INTENSITY control so that the trace is at a suitable viewing intensity.
5. Adjust the FOCUS control for the sharpest obtainable trace.
6. Adjust the CH1 Y POSITION control so that the lower edge of the trace is level with one of the two lower graticule lines.
7. Observe that the overall waveform occupies 6 full vertical divisions of the graticule.
8. Switch CH1 VOLTS/DIV switch to 0.1 V.
9. Observe now that the trace will only occupy 3 vertical division of the graticule.
10. Disconnect the input from CH1 INPUT leaving only a reference trace, which can be aligned with the graticule lines by using the TRACE ROTATION control.
11. Turn this trace off of the screen using the CH1 Y POSITION control.
12. Connect the input plug to CH2 INPUT.
13. Push the TRIG switch so that it releases to the outer position.
14. Switch on CH2 by rotating CH2 Y POSITION control clockwise until a click is heard. Further rotation will move the trace up the screen.
15. Set the lower edge of the trace to a suitable reference line and observe that the trace occupies 6 full vertical divisions.
16. By now the user will be conversant with the operation of the Y or vertical controls so now they should turn to the sweep controls. By turning the TIME/DIV control anti-clockwise in steps as far as it will go, it should be noticed that the sweep speed decreases.
17. Set the TIME/DIV knob to 1 ms and observe the sweep speed.
18. Set the TIME/DIV knob to 5 ms and note that the sweep should be slower.
19. Pull out the X5 control and observe that the sweep speeds should be the same as 17 above.

2.7 USE OF ADDITIONAL FACILITIES

2.7.1 TRIGGER SOURCE

We have been using the control in the INT position but it is possible to trigger from an external signal by plugging the signal into the EXT TRIG. socket (BNC) at the side of the instrument. The SOURCE switch should be set to EXT.

2.7.2 SLOPE

The SLOPE switch allows triggering from a positive (+) going or negative (−) going portion of the trigger signal. This is important when it is only required to observe a portion of a waveform but where several cycles of a waveform are displayed the setting is often unimportant.

2.7.3 MODE

For the inspection or measurement of most waveforms the MODE control is used in the AC position. For the inspection of TV frame or TV line waveforms the switch should be set to TV. For TV field waveforms sweep ranges of 0.5 sec/div to 0.1 ms/div should be used. For TV line waveforms sweep ranges of 50 μs/div to 0.5 μs/div are required.

2.7.4 LEVEL

There are two modes of level control operation. In the normal (control out) position the triggering point can be varied over the whole of the waveform to a maximum of 8 divisions and with a minimum sensitivity of 0.3 divisions.

In the AUTO position (control in) level control is restricted to approximately 1/8 of the normal variation. In the absence of a triggering waveform or if the waveform does not meet the required minimum sensitivity an automatic bright line reference trace is displayed.

2.8 BASIC APPLICATIONS

The following are typical applications of Oscilloscope type D32.

2.8.1 PEAK TO PEAK VOLTAGE MEASUREMENT – AC Symetrical waveform

1 Connect the waveform to be measured to CH1 or CH2 INPUT.

2 Set the appropriate VOLTS/DIV switch to display about 5 or 6 divisions of the waveform.

3 Set the AC/DC switch to AC.

4 Set the TIME/DIV switch to display several cycles of the waveform.

5 Use the Y POSITION control to set the lower edge of the waveform on one of the lower graticule lines and so that the top edge of the waveform is in the graticule area.

6 Estimate the vertical amplitude (div) of the signal on the screen.

7 Multiply the amplitude in 6 above by the VOLTS/DIV setting and by the attenuation factor of any probe used.

EXAMPLE

Assume a vertical deflection of 5.3 division using a X10 attenuation probe and a VOLTS/DIV setting of 0.05 Volts per division.

$$\therefore \text{Peak to Peak Voltage} = \text{Vertical deflection} \times \text{VOLTS/DIV (Setting)} \times \text{Attenuation factor (Probe)}$$

for our example

Peak to Peak voltage = 5.3 x 0.05 x 10

$\therefore$ Peak to Peak voltage = 2.65 Volts.

2.8.2 FREQUENCY MEASUREMENT

1 Connect the waveform to be measured, to CH1 or CH2 INPUT.

2 Set the VOLTS/DIV switch to display approximately 5 or 6 vertical divisions of the waveform.

3 Set the TIME/DIV control to display about 3 or 4 cycles of the waveform, keeping well inside the graticule limits.

4 Use the Y POSITION control to move the trace so that the start of each cycle is on the centre line.

5 The X POSITION control is used to move the start of 1 cycle to a convenient reference point.

6 Measure the distance (divs) between the start of the cycle and the end.

7 Multiply the measurement in 6 above by the setting of the TIME/DIV switch and if the X5 control is used divide by 5. This gives the time duration of 1 cycle.

8 In order to obtain the frequency it is necessary to take the reciprocal of the time duration found in 7.

EXAMPLE

If one cycle occupies 2.5 divisions with the TIME/DIV control on 0.2 ms/div and the magnifier is not used.

$$\text{Frequency} = \frac{1}{\text{horizontal distance} \times \text{TIME/DIV setting}}$$

$$\therefore \text{Frequency} = \frac{1}{2.5 \times 0.2 \text{ ms}}$$

$\therefore$ Frequency = 2 kHz.

SECTION 3
CIRCUIT DESCRIPTION

3.1 GENERAL

The D32 uses entirely solid state circuitry to drive a single beam cathode ray tube (CRT). Internal nickel cadmium cells supply a non-regulated invertor power unit. The cells are charged from a.c. lines via an internal line transformer and constant current charger. Field effect transistors (FETs) in the first stage of each vertical (Y) amplifier enable constant, high impedance inputs to be applied, whilst a further F.E.T. in the sawtooth generator ensures a high degree of ramp linearity.

Dual Y channel operation is achieved by alternate displays on a time sharing basis. At slow sweep speeds this is achieved by 'chopping' the waveforms and displaying portions of each waveform in turn during each sweep period. At higher sweep speeds the complete information on each channel is displayed on 'alternate' sweeps. The selection of 'Chop' or 'Alternate' is done automatically according to the setting of the TIME/DIV switch.

Normal triggering is a.c. coupled with selection of trigger point and polarity but an alternative mode allows triggering from a TV waveform. In both modes an 'AUTO' facility is provided whereby a bright line reference is displayed in the absence of a suitable triggering signal.

3.2 CHANNEL 1 & 2, Y AMPLIFIER AND ATTENUATOR

Reference to component numbers is 600 onwards for channel 1 and 700 onwards for channel 2, circuit operation for both channels being identical. Channel 1 operations will be described.

An input signal is fed into the BNC socket SK601 and fed to S601. In the A.C. position of the switch the signal is passed via C601 and in the D.C. position it is connected directly, to S602, the attenuator switch. The attenuator in addition to the straight through 1 : 1 range has four frequency — compensated resistive dividers, with ratios of 100 : 1, 10 : 1, 5 : 1 and 2 : 1.

These are switched singly or in tandem with C604, C605, C612 and C613 serving to standardise the input time constants. C602, C603, C606, C607, C608, C609, C611 and R610 provide compensation for the respective dividers. Basic input impedance is set by precision 1 MΩ resistor R609, shunted by capacity C616 which in addition to stray capacitance sets the basic channel input capacitance at high frequencies.

R611, C617 and low leakage diode D601 form an input protection circuit for the Field Effect Transistor TR601 connected as a source follower stage. Two signal outputs are provided from the FET. source, (1) a trigger signal to trigger select switch S623 and (2) vertical amplifier signal to TR603 at a DC level on or about ground, via R613. Main source load is R614. TR603 forms part of a long tailed pair amplifier with TR604. Emitter coupling diodes D602 and D603 provide the signal carrying capacity to provide close vertical amplifier gain tracking, with DC rail variation necessary to compensate for tube sensitivity variations. TR603 and TR604 tail resistors include trimmer R617 to initially set up amplifier gain and thermistor TH601 shunted by R625, to provide gain compensation with temperature. Thermal balance of TR603 and TR604 is provided by collector resistors R615 and R618, and H/F component of collector currents being shunted through capacitors C619 and C621.

Common base transistor TR602 buffers the collector of TR603 from post, chop/alternate switching waveforms thus isolating the trigger pick-off from these signals, which would lead to undesirable triggering effects.

3.3 VERTICAL OUTPUT AMPLIFIER figure 3

The collector currents of the selected channel pass through diodes D651 and D652 for Channel 1, or D657 and D658 for Channel 2, to the bases of shunt feedback stages TR651 and TR654. The outputs of TR651 and TR654 are fed to the bases of TR652 and TR653, a longtailed pair whose collectors feed the Y plates of the CRT. C655 and R657 in the emitter circuit are adjusted for the best fast pulse response. Channel 2 vertical amplifier can be switched on or off using S631 which is ganged to the CH2 Y POSITION control. With CH2 off the instrument is effectively a single channel instrument but when it is on the channels are selected for display by the CHOP/ALTERNATE circuit, TR631 and TR632. On TIME/DIV speeds of 2 ms/div and slower, TR631 and TR632 operate as a free running multivibrator at a frequency of approximately 100 kHz. When TR632 conducts, D653 and D654 conduct and turn off D651 and D652 thus disconnecting Channel 1. Conversely when TR631 conducts D655 and D656 conduct and turn off D657 and D658 thus disconnecting Channel 2. C632 and C637 feed pulses to the unblanking amplifier to blank out the trace during the transition. On Time/Div speeds above 2 ms/div, TR631 and TR632 operate as a bistable whose state is changed at the end of each timebase sweep by a negative going pulse from the collector of TR104. The network L631, C652, R648 in CH1 and L632, C656, R649 in CH2 delay the transitions until the trace is blanked.

3.4 TRIGGER CIRCUITS figure 4

The ac coupled trigger amplifier accepts either internal or external signals. Internal selection from either channel 1 or channel 2 being made by selector switch S632 to emitter follower TR633 and then by co-axial cable to C22. External trigger signals are applied via sockets SK21 and SK22 on the right hand side of the instrument and to the trigger amplifier via C21 and R21. Switch S21 selects EXT or INT. and S22 selects polarity before applying signals to the bases of amplifier pair TR21 and TR22. As all signals are derived from unbalanced sources the free transistor base is grounded with respect to ac via C23. The collector of TR22 is ac coupled via D23 to the base of TR23, a shunt feedback stage, whose input voltage excursion is limited by diodes D21, D22 and D23. C27, D24 and D25 attenuate high amplitude signals at H/F. The output of TR23 is fed to the Schmitt trigger circuit, TR25 and TR24, which provides a constant amplitude trigger signal to the timebase and bright line auto circuit on the AC position of S23. On the TV position of S23, TR25 is converted to a sync separator, and TR24 on TIME/DIV speeds slower than 100 μs has a long time constant in the emitter circuit, which provides positive differentiated field pulses of much greater amplitude than the line pulses and therefore the timebase tirggers on the field pulses. On TIME/DIV speeds faster than 100 μs, the emitter time constant is reduced by TR26 which short circuits R42, so that differentiated field and line pulses are of equal amplitude and the timebase therefore triggers at line frequency. In the AUTO position S24 switches in R40 to reduce effect of level potentiometer, permitting CRT displays greater than 1 div to be automatically triggered.

3.5 TIMEBASE, UNBLANKING AND BRIGHT LINE AUTO CIRCUIT figure 5

The differentiated positive pulse from the trigger circuit is fed via D101 to the base of TR102 which together with TR104 forms a bistable. The positive pulse turns on TR102 which in turn cuts off the clamping transistor TR101. The timebase, a

F.E.T. Miller circuit, then runs up linearly charging up the hold-off capacitor via R110 and D106 and resetting the bistable via R112. When TR102 switches off, TR101 conducts and discharges the timing capacitor until D103 conducts and reduces the current in TR101 to the value required by the timing resistor. At this point the flyback stops. During the flyback the hold-off capacitor discharges through R112 until D108 conducts, the circuit then "clamps" in a quiescent state and remains so until the arrival of the next triggering pulse.

If the Trig level control is in the Auto position and no trigger pulses are present, TR105 and D109 conduct and reduce the potential at the anode of D108. This allows the hold-off capacitor to discharge further and re-trigger the bistable. The timebase then free-runs. If trigger pulses are applied at the anode of D113 to TR106 base, TR106 then conducts during the period of the pulse, switching off TR105, via C106. TR105 collector potential then rises, back biasing D109 thus inhibiting the free run timebase sweep which is then dependant upon the trigger pulses.

The collector current of TR104 which is cut off during the sweep, is fed to the input of TR107. The collector of TR107 goes negative at the beginning of the sweep driving TR108 on, bringing the unblanking plate positive, and unblanking the trace. If the vertical channels are in the chopped mode the chop transitions are blanked via TR109 which pulls the unblanking plate negative in response to the chop blanking pulses fed to its base via C111. At the end of sweep, TR104 turns on, turning off TR107, TR108, and turning on TR109, returning the trace to the blanked condition.

Negative pulses from TR104 collector are fed to CHOP/ALT bistable to switch channels in the ALT mode at the end of each trace.

3.6 HORIZONTAL AMPLIFIER figure 5

TR111, TR112, TR113 and TR114 form a balanced symmetrical amplifier system to drive the CRT X plates.

Shunt feedback amplifier TR111 accepts sweep generator currents via R138 and a current from the horizontal position potentiometer R137 via R139. An output voltage proportional to the input currents is then applied to TR112 base. TR113 is longtailed with TR112 to form the output stage with X1 and X5 gain adjustment located between the emitters. Balance for TR113 is obtained from TR114, a similar stage to TR11., but with an effectively grounded input.

3.7 CATHODE RAY TUBE figure 6

V301 is a flat face, mesh cathode ray tube. The astigmatism electrode is fed from a low impedance supply, TR302, avoiding the necessity for re-adjustment of the astigmatism with change of brilliance.

Cathode-grid potential is stabilised by zener diode D303 and pre-set intensity control R309 takes up spread in tube characteristics. The geometry, mesh and focus electrodes are fed from a resistive divider which, with R313, provide bias currents for D303. A coil L301 is provided to take up variations in trace alignment with the graticule. It is fitted to the CRT neck, and supplied with a stabilised current, from TR301. The rear panel rotation control is in the base circuit of TR301. C303 and C304 provide inter plate decoupling to avoid unwanted Z modulation effects.

3.8 CALIBRATOR figure 6

Transistors TR315 and TR316 form a bistable switch, compensated against ambient temperature variations by D316 and D317, and supply stabilised by zener diode D315. Switch over is controlled by the sweep voltage applied via R315, to TR315. In the absence of sweep voltage, TR315 conducts and TR316 is switched off and DC voltage at SK315 is therefore zero. An increasing voltage applied to TR315 base reaches a level equal to TR316 base voltage, switch over then occurs, TR315 switches off and TR316 switches on. Collector current of TR316 determined by R316 and R318 then flows through precision resistor R323, providing a 300 mV DC output level to SK315. Switch over of TR315 and TR316 is arranged to occur at approximately half sweep, so that the CAL signal when applied to the Y amplifier, provides a zero volt datum level and a calibrated +300 mV level during the period of the sweep. R316 enables accurate setting of CAL voltage.

3.9 BATTERY CHARGER figure 7

Mains transformer T401 supplies current via fullwave rectifier D401 – D404, to TR401 and TR402 which provide a constant current charge to the batteries with the instrument switched off, or a trickle charge with the instrument on. Line voltage switching 100–125 V AC or 200–250 V AC is set by S401 located under the instrument via a small access hole, and connected to T401 primary. Range switching selecting the lower or upper 10% of each line voltage is set by S402 located at the rear of the instrument and is connected to T401 secondary. C402 smooths the rectified output. D405 and D406 stabilise TR401 base emitter voltage, bias current being provided by R401. TR401 with R402 in its emitter provides a constant current to the negative rail via D407 the "ON" panel LED. and part of R404. Forward bias voltage developed between R404 wiper and the negative rail causes TR402 to conduct and draw current from the positive rail via D408 and hence form the charge current for the battery pack. R404 therefore controls the charge current rate.

S403 and S404 form the 'ON' switch and are ganged together. Current demand in the 'ON' condition is over twice that in the 'OFF' condition, increased current is obtained from TR402 by switching in an additional parallel resistor R403. TR401 current is therefore increased, thereby increasing TR402 current. Battery charge rate in the 'OFF' condition is 400 mA and varies between zero and 100 mA in the 'ON' condition dependent upon actual line input voltage. D408 prevents battery discharge when instrument is stored.

3.10 CONVERTER POWER SUPPLY UNIT figure 7

All supply rails, with the exception of the battery charger, are derived from a push-pull, C.R. timed, DC to DC converter. TR411 and TR412 with protection diodes D411 and D412 drive ferrite cored transformer T411 at approximately 14 kHz, feedback being obtained from a single winding in series with C412 the timing capacitance. R411 and R412 are forward bias resistors decoupled by L411 and C411. C413 decouples supply lines from voltage spikes generated by switching action. +13 and –13 volt supplies are obtained from the two 14.5 volt windings on T411, rectified by D413, D414, D415 and D416 and smoothing is provided by R418, C418, L412 and C423 for +13 V and C421, L413 and C424 for –13 V.

An additional 23 volts winding added serially to a 14.5 V winding, rectified by D421 and smoothed by C422, L414 and C425 supplies +36 V. Additionally +80 V is obtained from the same windings by a voltage doubler C417, D418, D419 and C419.

CRT negative supplies for the gun are half wave rectified, from 523 volt winding, by D417 and smoothed by C415 and C416 in series.

PDA potential of 2.4 kV is obtained from the gun supply via a conventional quadrupler, comprising C431, C432, C433, C434, D431, D432, D433 and D434.

SECTION 4
MAINTENANCE AND CALIBRATION

DANGER

It is not possible to screen all high voltages, so care should be taken not to touch high voltage tags. Also where possible the instrument should be unplugged AND switched off during servicing. A BLEEDER PATH FOR THE EHT IS NOT PROVIDED, so before touching any internal parts the EHT should be discharged by temporarily shorting pin 13 on PC173 to chassis. It is advisable when replacing any component, or carrying out internal work, to disconnect the plug (PL402) and socket (SK402) at the top of the batteries to prevent an accidental short circuit from damaging the instrument.

4.1 INTRODUCTION

4.1.1 The solid state design of the instrument makes frequent adjustment of the internal preset components unnecessary. The appropriate part of the Calibration Procedure should be performed whenever the instrument fails to meet its specification, or whenever a defective component is replaced. The Circuit Description, Section 3, will assist in deciding which part of the circuit requires adjustment.

4.1.2 The internal 300 mV calibrator allows the accuracy of the vertical amplifiers to be checked. Timing accuracy should be checked against an external sinewave or marker pulse source.

4.1.3 To carry out the whole calibration procedure, the following tools and equipment are required:—

Small screwdriver (for access).

Trimming tool, low capacitance (for preset capacitors and potentiometers).

Amplitude calibrator, approximately 1 kHz squarewave providing outputs of 50 mV to 50 V. To an accuracy of ± 0.25%.

Time calibrator, providing markers of amplitude between 50 mV and 10 V, 1μsec. to 1 msec, timing accuracy ± 0.1%.

Squarewave generator, providing a terminated 1 MHz signal, of approximately 500 mV, rise time less than 10 nsec.

Sinewave generator, providing 50 kHz, to 10 MHz signal of amplitude up to 25 volts.

Monitor oscilloscope with X10 passive probe.

Digital voltmeter D.C. with input impedance of 1 meg ohm, or greater.

Composite TV video signal source.

Meter for voltage measurement with resistance of 20 kΩ per volt or better.

Ammeter 0.500 mA DC Accuracy ± 3%.

Co-Axial connecting leads and terminating load suitable for matching to co-as impedance.

X10 probe, available as equipment accessory.

4.2 MECHANICAL

4.2.1 ACCESS TO INTERIOR

a) Switch off LINE and instrument and remove all external leads and cables.
b) Follow the advice given in the Danger Warning.
c) Remove six screws securing rear cover.
d) Remove rear cover.
e) Hold case firmly, and push on rear chassis to withdraw the instrument through front of case.

4.2.2 OPENING OUT SIDE AND LOWER PANELS

(See exploded view)

a) Remove case as in 4.2.1 above.
b) To open the right hand panel loosen the screws at the top and bottom of the instrument just behind the Time/Div switch.
c) To open the left hand panel loosen the screws at the top and bottom of the instrument just behind the attenuators.
d) To open the bottom flap loosen the screw under the attenuator and the screw under the level potentiometer.

4.2.3 CRT REMOVAL

a) Remove instrument from case as in 4.2.1.
b) Through elongated hole in top rear chassis, slide back shield extension and carefully prise off tube base.
c) Stand instrument on rear chassis and open out side and bottom assemblies as 4.2.2
d) Break P.D.A. connector and earth each termination through 2MΩ resistor.
e) Unsolder trace rotate leads from eyelet numbers 6 & 7 on PC221.
f) Remove CRT shield securing screws located forward of battery packs.
g) Push CRT back to clear foam strips, and to unhook shield at top.
h) Lower face end of CRT and shield; withdraw both through lower opening.
j) Carefully separate the CRT and its shield.

4.2.4 CRT REFITTING

Follow the procedure 4.2.3 in reverse order, and make sure that CRT is pressed into the shield to locate against bezel rear before securing shield with its screws.
If trace rotation is in the opposite sense, reverse wires to eyelets 6 & 7, on PC221.

4.3 CALIBRATION PROCEDURE

4.3.1 BATTERY CHARGE RATE AND INITIAL SETTING

a) Ascertain actual A.C. line voltage available, and set range switch S401, located underneath and tapping switch, S402 on rear panel, as follows:—

AC LINE VOLTS	RANGE VOLTS (S401)	TAPPING (S402)
100-112 V	112 V	LO
113-125 V	112 V	HI
200-225 V	225 V	LO
226-250 V	225 V	HI

b) 1. Remove instrument chassis from case as in 4.2.1 above.
2. Open R.H. side assembly and remove one cell from battery pack.
3. Connect D.C. ammeter across cell holder contacts with ON/OFF switch set to off.
4. Connect instrument to A.C. line.
5. Adjust R404 on PC173 (underneath) for a current indication of 370 mA.
6. Disconnect a.c. line, remove ammeter, replace cell and secure side assembly.

c) Set front panel controls as follows:—
1. CH1 and CH2 AC/DC switches to AC.
2. CH1 and CH2 VOLT/DIV switches to 5 V/DIV.
3. Select CH1 trig.
4. CH1 position centralised, using Y POSITION knob.
5. CH2 position fully anti-clockwise to channel OFF position.
6. INTENSITY/Off to Off, focus centralised.
7. TIME/DIV to 1 ms horizontal position centralised and pushed to 'IN' position.
8. LEVEL, centralised, push in for 'AUTO'.
9. MODE, SOURCE and SLOPE switches set to AC, INT. and — respectively.

4.3.2 SUPPLY LINE VOLTAGES

Set controls as in para. 4.3.1, switch unit ON using intensity control. No adjustments exist for supply lines. The voltages shown in the table below are those which should be obtained for a nominal 7.8 volts battery pack voltage. (Measured between chassis and battery fuse using volt meter having resistance of 20 kΩ per volt). Allowance should be made for pack voltages differing from above. The under sub-assembly may be lowered to facilitate these measurements.

4.3.3 ASTIGMATISM AND GEOMETRY

a) Switch unit 'ON' and connect to AC line if batteries are in a low state of charge.
b) Set TIME/DIV to 20 μsec.
c) Apply 50 kHz sinewave signal to CH1 and set VOLTS/DIV for a 2 div p-p display.
d) Adjust LEVEL for stable trace.
e) Set trace equally about 2 horizontal lines from top of graticule.
f) Adjust FOCUS and R312 (Astigmatism) on PC173 for best trace definition.
g) Disconnect 50 kHz signal.
h) Set LEVEL to 'AUTO', trace should free run.
j) Set trace under centre graticule line, adjust trace rotate if necessary for best alignment.
k) Set trace under top horizontal line, adjust R302 (GEOMETRY) on PC173 for least curvature of trace.
l) After carrying out this adjustment the sweep accuracy should be checked, see para 4.3.8.

4.3.4 CH1 AND CH2 BALANCE

a) Set controls as para 4.3.1 (c).
b) Switch unit ON and display a free running trace.
c) Set CH1 POSITION control to half rotation.
d) Adjust R621 (CH1 BALANCE) PC187 to set trace to screen centre.
e) Set CH1 VOLTS/DIV switch to 10 mV.
f) Select DC and short circuit CH1 input socket, there should be no trace movement.
g) Apply 50 kHz sinewave to CH1 input and adjust amplitude for 8 vertical divisions display.
h) Adjust POSITION control from end to end note display overlaps.
j) Adjust R621 for equal peak overlap.
k) Repeat for CH2 using R721 (CH2 BALANCE).

4.3.5 CH1 AND CH2 GAIN AND ATTENUATOR

a) Select CH1, AC and 10 mV/DIV.
b) Switch unit ON and display a free-running trace (AUTO/LEVEL control IN).
c) Connect CH1 directly to 50 mV. 1 kHz squarewave calibrator.
d) Adjust R617 (CH1 GAIN) on PC187 for a 5 division amplitude display, neglecting any over, or under shoot.
e) Apply 500 mV 1 kHz squarewave to CH1 via 10 : 1 probe and adjust probe compensation for squarest corner and flat top on display then remove probe.
f) Set CH1 to 20 mV, apply 100 mV 10 kHz squarewave, adjust C611 for squarest corner and flat top.
g) Apply 1 volt 10 kHz via 10 : 1 probe, adjust C612 only for squarest corner and flat top on display, then remove probe.
h) Set CH1 to 50 mV/div, apply a 250 mV 10 kHz signal and adjust C615 for squarest corner and flat top.
j) Apply 2.5 V 10 kHz signal via 10 : 1 probe and adjust C613 for squarest corner and flat top then remove probe.
k) Set CH1 to 0.1 V/div, apply 0.5 V 10 kHz signal and adjust C603 for squarest corner and flat top.
l) Apply 5 V 10 kHz signal via 10 : 1 probe, adjust C604 for squarest corner and flat top then remove probe.
m) Set CH1 to 1.0 V, apply 5 V 10 kHz signal adjust C608 for squarest corner and flat top.
n) Apply 50 V 10 kHz via 10 : 1 probe, adjust C605 for squarest corner and flat top then remove probe.
p) Apply squarewave from calibrator to each of the nine V/div settings in turn and check for square response and amplitude error, which should not exceed 5%.
q) Repeat above for CH2 using appropriate trimmers which are prefixed with a 7. e.g. R617 for CH1 becomes R717 for CH2 etc.

TABLE OF EXPECTED VOLTAGES

SUPPLY LINE	TEST POINT	P.C. BOARD	LIMITS
+7.5 V	Lower end of D301	PC187	+7.1 V to +7.9 V
+13 V	Eyelet No. 46	PC187	+12.65 V to +14 V
+36 V	Positive lead of C425	PC187	+35 V to +41 V
+80 V	Junction C419, D419	PC173	+78 V to +86 V
+2400 V	Eyelet No. 13	PC173	+2.2 kV to +2.43 kV
−560 V	Neg. lead of C416	PC173	−540 V to −600 V
−13 V	Forward lead of L413	PC187	−12.9 V to −14.5 V
−7.5 V	Lower end of D302	PC187	−7.2 V to −7.95 V

4.3.6 CH1 AND CH2 HF PULSE RESPONSE

a) Set controls as in para 4.3.1 but with both VOLTS/DIV switches set to 0.05 V.
b) Apply 1 MHz square wave signal to both channels simultaneously via cable terminating load.
c) Switch unit on and switch CH2 on.
d) Set TIME/DIV switch to 0.5 μsec.
e) Display 5 div signal of CH1 and adjust R657 and C655 on PC187 for squarest leading/top edge of display. (x5 horizontal gain may be used to facilitate this).
f) Display CH2 and adjust R657 and C655 for best compromise, a 3 per cent overshoot or ring on the leading corner is permissible.
g) The 10 MHz channel response may now be checked, from a 50 kHz, 5 division datum point at all settings of V/DIV switches 3db = >10 MHz.

4.3.7 SWEEP ACCURACY

a) Set controls as in para 4.3.1.
b) Apply 1 m sec. time markers to CH1.
c) Switch unit on.
d) Adjust level for most stable display.
e) Adjust R152 (x1 gain) on PC172, in conjunction with horizontal position control for an accurate marker/graticule alignment of 1 : 1.
f) Pull horizontal position control for x5 gain and adjust R151 (x5 gain) on PC172, and horizontal position control for an accurate marker/graticule alignment of 1 : 5.
g) Set TIME/DIV to 0.5 μsec. set horizontal position to x1 gain, apply 1 μsec. markers, adjust C2, trimmer capacitor on TIME/DIV switch, and horizontal position control for an accurate marker/graticule alignment of 1 : 2.

4.3.8 TRIGGER SENSITIVITY

a) Set controls as in para 4.3.1 but with TIME/DIV set to 10 μsec.
b) Apply 50 kHz sinewave signal to CH1 input.
c) Connect x10 probe of monitor oscilloscope to upper end of R32 or R33 on PC172.
d) Switch unit on.
e) Set monitor scope sensitivity to 10 mV/div and adjust 50 kHz input to display approximately 6 div. on monitor.
f) Adjust level until switching transients appear on monitor display. See waveform below.
g) Adjust R36 (backlash) on PC172 until transients are separated by 1.5 div vertically (or 150 mV at probe tip). Disconnect probe and monitor.

4.3.9 SWEEP STABILITY AND LENGTH

a) Set controls as in para 4.3.1 but with LEVEL control in 'OUT' position and fully clockwise.
b) Switch unit on.
c) Adjust R116 (stability) on PC172 until trace appears then back off R116 until trace just ceases.
d) Note position of R116 rotor.
e) Apply 50 kHz sinewave signal to CH1 input.
f) Set TIME/DIV to 10 μsec.
g) Adjust level for a stable display.
h) Back off R116 until trace disappears and note R116 rotor position.
j) Set R116 mid way between two noted positions.
k) Adjust R107 (sweep length) on PC172 for a trace length of 10.2 divisions.

4.3.10 INTERNAL CALIBRATOR

a) Set controls as in para 4.3.1 but with TIME/DIV set to 0.5 sec.
b) Set CH1 attenuator to 0.1 V and DC.
c) Connect CAL output to CH1 input and to digital voltmeter.
d) Connect ground of digital voltmeter to ground socket on R.H. side.
e) Switch unit on and note that trace steps upwards, approximately half way across screen.
f) Note digital volt meter reading after step has taken place, and adjust R316 (calibrator) on PC172 for a reading of 300 mV ±0.3 mV.

4.3.11 TV TRIGGER

a) Select CH1, DC, TV, INT and +ve polarity.
b) Apply composite T.V. video signal to CH1, and adjust amplitude of CH1 attenuator for a 3 division p-p display.
c) By adjustment of LEVEL control, in the 'OUT' position only, TV line synchronisation should occur on the seven fastest sweep ranges, and TV field on the twelve slowest ranges. There are no internal adjustments for T.V. and failure to lock would indicate a circuit fault.

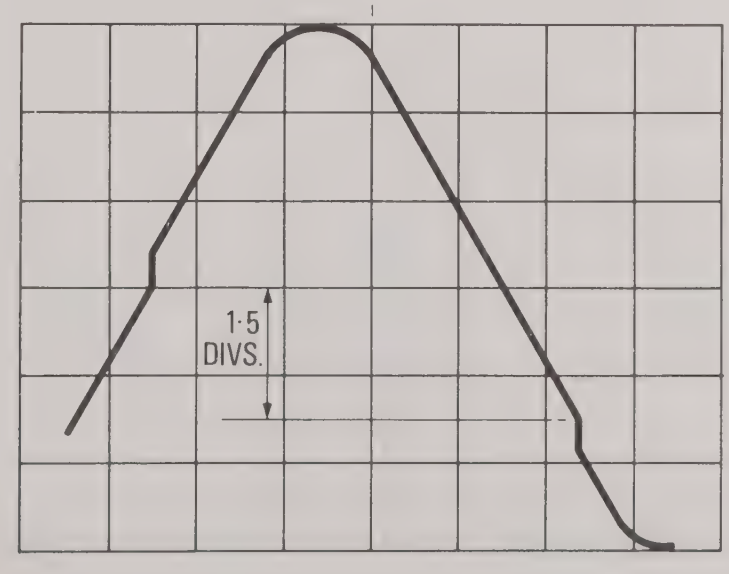

SECTION 5
COMPONENTS LIST

Values of resistors are stated in ohms or multiples of ohms; ratings at 70°C are in watts or sub-multiples of watts. Values of capacitors are stated in sub-multiples of farads; ratings at 70°C are in volts or kilovolts.

Whenever possible, exact replacements for components should be used, although locally available alternatives may be satisfactory for standard components.

Any order for replacement parts should include:

1. Instrument type
2. Instrument serial number
3. Component circuit reference
4. Component part number
5. Component value

CIRCUIT REFERENCE BLOCKS

The table below gives the blocks of circuit references, so that the reader can relate the items listed in this chapter and their location in the circuitry in Section 6.

Circuit Reference		Circuit	Fig.
From	To		
1	300	Sweep Generator, Unblanking & X Amp. Time/Div Switch Trigger	5 8 4
301	400	Calibrator & CRT	6
401	600	Battery Charger Power Supply	7
601	630	Channel 1 Input	1
631	700	Y Output Chop-Alternate Bistable	3
701	730	Channel 2 Input	2

ABBREVIATIONS

BM	Button mica	CMP	Cermet preset	PS	Polystyrene
C	Carbon	E	Electrolytic	Se	Selenium
CP	Carbon preset	Ge	Germanium	Si	Silicon
CV	Carbon variable	MF	Metal Film	SM	Silver mica
CER	Ceramic	MO	Metal oxide	WW	Wire-wound
CT	Ceramic Trimmer	PC	Polycarbonate	WWP	Wire-wound preset
CM	Cermet thick film	PE	Polyester	WWV	Wire-wound variable
		PP	Polypropylene		

TEKTRONIX U.K. LIMITED

36 - 38 Coldharbour Lane, Harpenden, Hertfordshire, England

Telephone: Harpenden 63141 Telex: 25559

All requests for repairs or replacement parts should be directed to the Tektronix Field Office or representative in your area. In the UK contact the Harpenden address above. This procedure will assure you the fastest possible service.

CIR REF	PART NUMBER	VALUE	DESCRIPTION	RATING	Eff Ser.No.
B401	146-0027-00	1.25 V	Cell Ni Cad. D Size	4AH	
B402	146-0027-00	1.25 V	Cell Ni Cad. D Size	4AH	
B403	146-0027-00	1.25 V	Cell Ni Cad. D Size	4AH	
B404	146-0027-00	1.25 V	Cell Ni Cad. D Size	4AH	
B405	146-0027-00	1.25 V	Cell Ni Cad. D Size	4AH	
B406	146-0027-00	1.25 V	Cell Ni Cad. D Size	4 AH	

CIR REF	PART NUMBER	VALUE F	DESCRIPTION TYPE	TOL %	RATING Volts	Eff. Ser.No.
C1	285-0786-00	33p	PS	2 p	350	703301
C2	281-0732-00	3 - 12 p	CT		350	703101
C3	285-1110-00	1.0 μ	PC	1	40	
C4	285-1146-00	10 n	PS	1	63	611501
C5	285-1057-00	30 p	PS	1 p	350	
C6	285-0828-00	22 n	PE	5	250	612001
C7	285-1078-00	1.5 μ	PE	20	63	
C8	281-0710-00	10 n	CER		250	
C9	281-0710-00	10 n	CER		250	
C21	285-0796-00	100 n	PE	20	250	
C22	290-0493-00	22 μ	ELEC		25	
C23	285-0915-00	100 n	PE	20	100	
C24	281-0710-00	10 n	CER		250	
C25	290-0943-00	22 μ	ELEC		25	
C27	285-0854-00	100 p	PS	2 p	350	
C28	290-0661-00	100 μ	ELEC		16	
C29	290-0661-00	100 μ	ELEC		16	
C31	285-0869-00	47 p	PS	2 p	350	
C32	285-0854-00	100 p	PS	2 p	350	
C33	290-0762-00	22 μ	ELEC		6.3	609351
C34	285-0759-00	2.2 n	PS	5	125	
C35	285-0887-00	1.5 n	PS	5	125	
C36	290-0707-00	22 μ	ELEC		25	
C37	285-0869-00	47 p	PS	2 p	350	
C100	285-0871-00	150 p	PS	5	350	
C101	285-0776-00	27 p	PS	1 p	350	
C102	290-0661-00	100 μ	ELEC		16	
C103	281-0710-00	10 n	CER		250	
C104	285-1054-00	270 p	PS	1	350	609280
C105	285-0867-00	20 p	PS	1 p	350	
C106	285-0779-00	470 n	PE	20	100	
C107	290-0623-00	4.7 μ	ELEC		25	
C108	285-1018-00	22 p	PS	1 p	350	
C109	281-0705-00	1 p	CER	0 1 p	500	
C110	285-0915-00	100 n	PE	20	100	
C111	285-0847-00	560 p	PS	5	125	
C112	285-0915-00	100 n	PE	20	100	
C113	285-0915-00	100 n	PE	20	100	
C114	281-0711-00	3.9 p	CER	0.25 p	750	609151
C115	285-0867-00	20 p	PS	1 p	350	
C116	285-0873-00	200 p	PS	5	350	610002
C301	281-0710-00	10 n	CER		250	
C302	281-0710-00	10 n	CER		250	
C303	281-0710-00	10 n	CER		250	
C304	281-0710-00	10 n	CER		250	
C305	281 0710-00	10 n	CER		250	609249

CIR REF	PART NUMBER	VALUE F	DESCRIPTION TYPE	TOL %	RATING Volts	Eff. Ser.No.
C402	290-0675-01	4.7 m	ELEC		16	
C403	285-0915-00	100 n	PE	20	100	
C411	290-0676-00	1 μ	ELEC		100	
C412	285-0836-00	47 n	PE	20	250	
C413	290-0679-00	1 m	ELEC		10	
C415	290-0677-00	1 μ	ELEC		350	
C416	290-0677-00	1 μ	ELEC		350	
C417	290-0676-00	1 μ	ELEC		100	
C418	290-0678-00	47 μ	ELEC		25	
C419	290-0676-00	1 μ	ELEC		100	
C421	290-0678-00	47 μ	ELEC		25	
C422	290-0688-00	22 μ	ELEC		63	
C423	290-0678-00	47 μ	ELEC		25	
C424	290-0678-00	47 μ	ELEC		25	
C425	290-0688-00	22 μ	ELEC		63	
C431	281-0747-00	1.8 n	CER		1250	
C432	281-0747-00	1.8 n	CER		1250	
C433	281-0748-00	1 n	CER	20	1250	
C434	281-0748-00	1 n	CER	20	1250	
C601	285-0796-00	100 n	PE	20	250	
C602	281-0723-00	1.8 p	CER	0.1 p	500	
C603	281-0155-00	2-22 p	PS		500	
C604	281-0155-00	2-22 p	PS		500	
C605	281-0155-00	2-22 p	PS		500	
C606	Twisted wires mounted on S602					
C607	285-1080-00	220 p	PS	5	350	
C608	281-0157-00	5.5-65.5 p	PS		500	
C609	285-0776-00	27 p	PS	1 p	350	
C611	281-0154-00	2-12 p	PS		500	
C612	281-0156-00	1.4-6.4 p	PS		500	
C613	281-0155-00	2-22 p	PS		500	
C614	281-0731-00	5.6 p	CER	0.5 p	750	
C615	281-0155-00	2-22 p	PS		500	
C616	281-0731-00	5.6 p	CER	0.5 p	750	
C617	281-0710-00	10 n	CER		250	
C618	285-0915-00	100 n	PE	20	100	
C619	285-0887-00	1.5 n	PS		125	
C621	285-0759-00	2.2 n	PS	5	125	
C622	285-0760-00	330 p	PS	5	125	

CIR REF	PART NUMBER	VALUE F	DESCRIPTION TYPE	TOL %	RATING Volts	Eff. Ser.No.
C631	285-0915-00	100 n	PE	20	100	
C632	285-0850-00	1000 p	PS	5	125	
C633	285-0760-00	330 p	PS	5	125	
C634	285-0845-00	68 pf	PS	2 p	350	703301
C635	285-0800-00	10 n	PE	20	250	
C636	285-0760-00	330 p	PS	5	125	
C637	285-0850-00	1000 p	PS	5	125	
C638	*285-0845-00	68 p	PS	2 p	350	703301
C651	281-0710-00	10 n	CER		250	
C652	285-0872-00	180 p	PS	2	350	703301
C653	281-0676-00	2.2 p	CER	0.1 p	500	
C654	281-0676-00	2.2 p	CER	0.1 p	500	
C655	281-0157-00	5.5-65.5 p			500	
C656	285-0872-00	180 p	PS	2	350	703301
C657	281-0710-00	10 n	CER		250	
C658	290-0623-00	4.7 µ	ELEC		25	
C659	290-0707-00	22 µ	ELEC		25	
*C660	285-0844-00	39 p	PS	2 p	350	609249
C661	285-0920-00	56 p	PS	2 p	350	609249

CIR REF	PART NUMBER	VALUE F	DESCRIPTION TYPE	TOL %	RATING Volts	Eff. Ser.No.
C701	285-0796-00	100 n	PE	20	250	
C702	281-0723-00	1.8 p	CER	0.1 p	500	
C703	281-0155-00	2-22 p	PS		500	
C704	281-0155-00	2-22 p	PS		500	
C705	281-0155-00	2-22 p	PS		500	
C706	Twisted wires mounted on S702					
C707	285-1080-00	220 p	PS	5	350	
C708	281-0157-00	5.5-65.5 p	PS		500	
C709	285-0776-00	27 p	PS	1 p	350	
C711	281-0154-00	2-12 p	PS		500	
C712	281-0156-00	1.4-6.4 p	PS		500	
C713	281-0155-00	2-22 p	PS		500	
C714	281-0731-00	5.6 p	CER	0.5 p	750	
C715	281-0155-00	2-22 p	PS		500	
C716	281-0731-00	5.6 p	CER	0.5 p	750	
C717	281-0710-00	10 n	CER		250	
C719	285-0887-00	1.5 n	PS		125	
C721	285-0759-00	2.2 n	PS	5	125	
C722	285-0760-00	330 p	PS	5	125	

* not fitted on some instruments.

CIR REF	PART NUMBER	VALUE	DESCRIPTION	TYPE	TOL %	RATING	Eff. Ser.No.
D21	152-0062-01	75 V	1N914	Si		50 mA	
D22	152-0062-01	75 V	1N914	Si		50 mA	
D23	152-0062-01	75 V	1N914	Si		50 mA	
D24	152-0370-00	50 V	AAY30	Ge		25 mA	
D25	152-0370-00	50 V	AAY30	Ge		25 mA	
D101	152-0062-01	75 V	1N914	Si		50 mA	
D102	152-0062-01	75 V	1N914	Si		50 mA	
D103	152-0062-02	75 V	1N4148T	Si		50 mA	609280
D104	152-0062-01	75 V	1N914	Si		50 mA	
D105	152-0062-01	75 V	1N914	Si		50 mA	
D106	152-0062-01	75 V	1N914	Si		50 mA	
D107	152-0062-01	75 V	1N914	Si		50 mA	
D108	152-0062-01	75 V	1N914	Si		50 mA	
D109	152-0062-01	75 V	1N914	Si		50 mA	
D111	152-0062-01	75 V	1N914	Si		50 mA	
D112	152-0062-01	75 V	1N914	Si		50 mA	
D113	152-0062-01	75 V	1N914	Si		50 mA	
D114	152-0062-01	75 V	1N914	Si		50 mA	611501
D115	152-0062-01	75 V	1N914	Si		50 mA	611501
D301	152-0347-00	7.5 V	Zener	Si		330 mW	
D302	152-0347-00	7.5 V	Zener	Si		330 mW	
D303	152-0388-00	130 V	Zener	Si		400 mW	
D304	152-0062-01	75 V	1N914	Si		50 mA	
D315	152-0347-00	7.5 V	Zener	Si		330 mW	
D316	152-0062-01	75 V	1N914	Si		50 mA	
D317	152-0062-01	75 V	1N914	Si		50 mA	

CIR REF	PART NUMBER	VALUE	DESCRIPTION	TYPE	TOL %	RATING	Eff. Ser.No.
D401	152-0339-00		1N4001	Si		50 V	
D402	152-0339-00		1N4001	Si		50 V	
D403	152-0339-00		1N4001	Si		50 V	
D404	152-0339-00		1N4001	Si		50 V	
D405	152-0421-00	3.3 V	Zener	Si		330 mW	
D406	152-0062-01	75 V	1N914	Si		50 mA	
D407	152-0625-01		L.E.D.	Ga Asp		50 mA	613251
D408	152-0467-00		1N5400	Si		50 V	
D411	152-0062-01	75 V	1N914	Si		50 mA	
D412	152-0062-01	75 V	1N914	Si		50 mA	
D413	152-0468-00		BAX16	Si		150 V	
D414	152-0468-00		BAX16	Si		150 V	
D415	152-0468-00		BAX16	Si		150 V	
D416	152-0468-00		BAX16	Si		150 V	
D417	152-0515-00		SCM60	Si		6 kV	
D418	152-0468-00		BAX16	Si		150 V	
D419	152-0468-00		BAX16	Si		150 V	
D421	152-0468-00		BAX16	Si		150 V	
D431	152-0515-00		SCM60	Si		6 kV	
D432	152-0515-00		SCM60	Si		6 kV	
D433	152-0515-00		SCM60	Si		6 kV	
D434	152-0515-00		SCM60	Si		6 kV	
D601	152-0483-00	10 V	CE1104	Si			
D602	152-0541-00	12 V	BAY 82	Si		50 mA	610101
D603	152-0541-00	12 V	BAY 82	Si		50 mA	610101
D631	152-0062-01	75 V	1N914	Si		50 mA	
D632	152-0062-01	75 V	1N914	Si		50 mA	
D633	152-0062-01	75 V	1N914	Si		50 mA	
D634	152-0062-01	75 V	1N914	Si		50 mA	
D635	152-0062-01	75 V	1N914	Si		50 mA	
D636	152-0062-01	75 V	1N914	Si		50 mA	612401
D651	152-0614-00	40 V	1N4448	Si		75 mA	611501
D652	152-0614-00	40 V	1N4448	Si		75 mA	611501
D653	152-0614-00	40 V	1N4448	Si		75 mA	611501
D654	152-0614-00	40 V	1N4448	Si		75 mA	611501
D655	152-0614-00	40 V	1N4448	Si		75 mA	611501
D656	152-0614-00	40 V	1N4448	Si		75 mA	611501
D657	152-0614-00	40 V	1N4448	Si		75 mA	611501
D658	152-0614-00	40 V	1N4448	Si		75 mA	611501
D659	152-0625-01		L E.D.	Ga Asp			613251
D701	152-0483-00	10 V	CE1104	Si			
D702	152-0541-00	12 V	BAY 82	Si		50 mA	610101
D703	152-0541-00	12 V	BAY 82	Si		50 mA	610101

CIR REF	PART NUMBER	VALUE	DESCRIPTION	TYPE	TOL %	RATING	Eff. Ser.No.
FB601	276-0597-00		Ferrox Cube Bead FX1115				609201
FB701	276-0597-00		Ferrox Cube Bead FX1115				609201
FS401	159-0079-00	500 mA	Fuse Link 1.25" lg. slow (for 112V)				
FS401	159-0077-00	250 mA	Fuse Link 1.25" lg. slow (for 225V)				
FS402	159-0076-00	3 A	Fuse Link 1.25" lg. slow(battery)				
L301	(with V301)		Trace Rotation Coil				
L402	108-0837-00	100 μH	Inductor fixed Ferrite cored		5		610101
L411	108-0482-00	160 μH	Inductor fixed Iron dust cored				
L412	108-0482-00	160 μH	Inductor fixed Iron dust cored				
L413	108-0482-00	160 μH	Inductor fixed Iron dust cored				
L414	108-0482-00	160 μH	Inductor fixed Iron dust cored				
L631	108-0780-00	53 μH	Inductor Iron dust cored		10		
L632	108-0780-00	53 μH	Inductor Iron dust cored		10		
L633	108-0482-00	160 μH	Inductor Iron dust cored				
L634	108-0482-00	160 μH	Inductor Iron dust cored				
PL401	134-0154-00		Plug — Mains				
PL402	134-0125-00		Plug — Charging check				

CIR REF	PART NUMBER	VALUE Ohms	DESCRIPTION TYPE	TOL %	RATING Watts	Eff. Ser.No.
R1	325-0166-00	143 k	MF	1	250 m	
R2	325-0166-00	143 k	MF	1	250 m	
R3	325-0167-00	422 k	MF	1	250 m	
R4	325-0168-00	715 k	MF	1	500 m	
R5	325-0169-00	1.43 M	MF	1	500 m	
R6	325-0170-00	4.22 M	MF	1	500 m	
R20	317-0180-01	18	C	5	125 m	
R21	317-0513-01	51k	C	5	125 m	610841
R22	317-0561-01	560	C	5	125 m	
R23	317-0682-01	6.8 k	C	5	125 m	
R24	317-0622-01	6.2 k	C	5	125 m	
R25	317-0682-01	6.8 k	C	5	125 m	
R26	317-0561-01	560	C	5	125 m	
R27†	311-1708-00	47 k	CV	20	250 m	
R28	317-0393-01	39 k	C	5	125 m	
R29	317-0273-01	27 k	C	5	125 m	
R30	317-0180-01	18	C	5	125 m	

† with switch

CIR REF	PART NUMBER	VALUE Ohms	DESCRIPTION TYPE	TOL %	RATING Watts	Eff. Ser.No.
R31	317-0563-01	56 k	C	5	125 m	
R32	317-0682-01	6.8 k	C	5	125 m	
R33	317-0362-01	3.6 k	C	5	125 m	
R34	317-0101-01	100	C	5	125 m	
R35	317-0622-01	6.2 k	C	5	125 m	609351
R36	311-1893-00	100	CMP	20	500 m	611101
R37	317-0201-01	200	C	5	125 m	
R38	317-0121-01	120	C	5	125 m	
R39	317-0392-01	3.9 k	C	5	125 m	
R40	317-0105-01	1 M	C	5	125 m	
R41	317-0103-01	10 k	C	5	125 m	
R42	317-0334-01	330 k	C	5	125 m	
R43	317-0753-01	75 k	C	5	125 m	
R44	317-0331-01	330	C	5	125 m	
R45	317-0104-01	100 k	C	5	125 m	
R46	317-0105-01	1 M	C	5	125 m	
R47	317-0752-01	7.5 k	C	5	125 m	609351
R48	317-0101-01	100	C	5	125 m	
R49	317-0182-01	1.8 k	C	5	125 m	
R50	311-1692-00	22 k	CP	20	50 m	
R51	317-0821-01	820	C	5	125 m	
R52	317-0470-01	47	C	5	125 m	

CIR REF	PART NUMBER	VALUE Ohms	DESCRIPTION TYPE	TOL %	RATING Watts	Eff. Ser.No.
R101	317-0203-01	20 k	C	5	125 m	
R102	317-0332-01	3.3 k	C	5	125 m	
R103	317-0332-01	3.3 k	C	5	125 m	
R104	317-0823-01	82 k	C	5	125 m	611801
R105	317-0103-01	10 k	C	5	125 m	
R106	317-0752-01	7.5 k	C	5	125 m	609280
R107	311-1692-00	22 k	CP	20	50 m	
R108	317-0471-01	470	C	5	125 m	
R109	317-0471-01	470	C	5	125 m	
R110	317-0621-01	620	C	5	125 m	
R111	317-0622-01	6.2 k	C	5	125 m	
R112	317-0203-01	20 k	C	5	125 m	612001
R113	317-0913-01	91 k	C	5	125 m	
R114	317-0123-01	12 k	C	5	125 m	
R115	317-0153-01	15 k	C	5	125 m	
R116	311-1654-00	10 k	CP	20	50 m	
R117	317-0103-01	10 k	C	5	125 m	
R118	317-0223-01	22 k	C	5	125 m	
R119	317-0391-01	390	C	5	125 m	
R121	317-0123-01	12 k	C	5	125 m	
R122	317-0564-01	560 k	C	5	125 m	
R123	317-0753-01	75 k	C	5	125 m	
R124	317-0822-01	8.2 k	C	5	125 m	
R125	317-0432-01	4.3 k	C	5	125 m	
R126	317-0123-01	12 k	C	5	125 m	
R127	317-0331-01	330	C	5	125 m	
R128	317-0123-01	12 k	C	5	125 m	
R129	317-0623-01	62 k	C	5	125 m	
R131	317-0222-01	2.2 k	C	5	125 m	
R132	317-0103-01	10 k	C	5	125 m	
R133	317-0334-01	330 k	C	5	125 m	
R134	317-0220-01	22	C	5	125 m	
R135	317-0332-01	3.3 k	C	5	125 m	
R136	317-0822-01	8.2 k	C	5	125 m	
R137†	311-1648-00	22 k	CV	20	250 m	
R138	317-0333-01	33 k	C	5	125 m	
R139	317-0363-01	36 k	C	5	125 m	
R141	317-0223-01	22 k	C	5	125 m	
R142	317-0123-01	12 k	C	5	125 m	
R143	317-0103-01	10 k	C	5	125 m	
R144	317-0622-01	6.2 k	C	5	125 m	
R145	317-0330-01	33	C	5	125 m	
R146	317-0562-01	5.6 k	C	5	125 m	
R147	317-0272-01	2.7 k	C	5	125 m	
R148	317-0101-01	100 R	C	5	125 m	
R149	317-0471-00	470	C	5	125 m	
R151	311-1655-00	100	CP	20	50 m	
R152	311-1706-00	470	CP	20	50 m	
R153	317-0752-01	7.5 k	C	5	125 m	
R154	317-0362-01	3.6 k	C	5	125 m	
R155	317-0330-01	33	C	5	125 m	
R156	317-0622-01	6.2 k	C	5	125 m	
R157	317-0103-01	10 k	C	5	125 m	
R158	317-0103-01	10 k	C	5	125 m	
R301	317-0241-01	240	C	5	125 m	
R302	311-1649-00	470 k	CP	20	50 m	
R303	311-1776-00	47 k	CV	20	100 m	
R304	317-0241-01	240	C	5	125 m	
R305	301-0565-01	5.6 M	C	5	500 m	
R306†	311-1816-00	1 M	CV	20	150 m	609451
R307	316-0185-01	1.8 M	C	10	250 m	609351

† with switch

CIR REF	PART NUMBER	VALUE Ohms	DESCRIPTION TYPE	TOL	RATING Watts	Eff. Ser.No.
R308†	311-1816-00	1 M	CV	20	150 m	609451
R309	311-1651-00	1 M	CP	20	50 m	
R310	317-0824-01	820 k	C	5	125 m	
R311	317-0105-01	1 M	C	5	125 m	
R312	311-1651-00	1 M	CP	20	50 m	
R313	315-0105-02	1 M	C	5	250 m	
R314	317-0272-01	2.7 k	C	5	125 m	
R315	317-0104-01	100 k	C	5	125 m	
R316	311-1652-00	2.2 k	CP	20	50 m	
R317	317-0104-01	100 k	C	5	125 m	
R318	317-0682-01	6.8 k	C	5	125 m	
R319	317-0222-01	2.2 k	C	5	125 m	
R321	317-0333-01	33 k	C	5	125 m	
R322	317-0433-01	43 k	C	5	125 m	
R323	321-0172-48	604	MF	1	125 m	
R324	317-0222-01	2.2 k	C	5	125 m	
R401	317-0152-01	1.5 k	C	5	125 m	
R402	317-0181-01	180	C	5	125 m	
R403	317-0151-01	150	C	5	125 m	
R404	311-1653-00	220	CP	20	50 m	
R405	308-0727-00	1	WW	10	1	
R406	317-0104-00	100 k	C	5	125 m	
R411	317-0102-01	1 k	C	5	125 m	
R412	317-0102-01	1 k	C	5	125 m	
R413	317-0241-01	240	C	5	125 m	
R414	317-0241-01	240	C	5	125 m	
R415	317-0102-01	1 k	C	5	125 m	
R416	317-0102-01	1 k	C	5	125 m	
R417	317-0102-01	1 k	C	5	125 m	
R418	307-0382-00	7.5	C	5	125 m	
R601 *	310-0679-00	900 k		1	250 m	
R602 *		111 k		1	250 m	
R603 *	310-0678-00	990 k		1	250 m	
R604 *		10.1 k		1	250 m	
R605 *		500 k		1	250 m	
R606 *		1 M		1	250 m	
R607 *	310-0683-00	800 k		1	250 m	
R608 *		250 k		1	250 m	
R609 *		1 M		1	250 m	
R610	317-0150-01	15	C	5	125 m	612101
R611	315-0104-01	100 k	C	5	250 m	
R612	317-0101-01	100	C	5	125 m	
R613	317-0750-01	75	C	5	125 m	
R614	317-0152-01	1.5 k	C	5	125 m	
R615	317-0332-01	3.3 k	C	5	125 m	
R616	317-0113-01	11 k	C	5	125 m	609351
R617	311-1656-00	4.7 k	CP	5	50 m	
R618	317-0912-01	9.1 k	C	5	125 m	
R619	317-0102-01	1 k	C	5	125 m	
R621	311-1764-00	47 k	CMP	20	500 m	
R622	317-0203-01	20 k	C	5	125 m	
R623	311-1658-00	47 k	CV	20	250 m	
R624	317-0913-01	91 k	CF	5	125 m	612301
R625	317-0302-01	3 k	C	5	125 m	

* thick film cermet resistor

CIR REF	PART NUMBER	VALUE Ohms	DESCRIPTION TYPE	TOL %	RATING Watts	Eff. Ser.No.
R631	317-0103-01	10 k	C	5	125 m	
R632	317-0151-01	150	C	5	125 m	
R633	317-0361-01	360	C	5	125 m	
R634	317-0752-01	7.5 k	C	5	125 m	
R635	317-0153-01	15 k	C	5	125 m	
R636	317-0223-01	22 k	C	5	125 m	
R637	317-0103-01	10 k	C	5	125 m	
R638	317-0512-01	5.1 k	C	5	125 m	
R639	317-0223-01	22 k	C	5	125 m	
R640	317-0153-01	15 k	C	5	125 m	
R641	317-0821-01	820	C	5	125 m	
R642	317-0392-01	3.9 k	C	5	125 m	
R643	317-0512-01	5.1 k	C	5	125 m	
R644	317-0153-01	15 k	C	5	125 m	
R645	317-0361-01	360	C	5	125 m	
R646	317-0752-01	7.5 k	C	5	125 m	
R647	317-0103-01	10 k	C	5	125 m	
R648	317-0102-01	1 k	C	5	125 m	
R649	317-0102-01	1 k	C	5	125 m	
R650	317-0473-01	47k	CF	5	125 m	612401
R651	317-0152-01	1.5 k	C	5	125 m	
R652	317-0752-01	7.5 k	C	5	125 m	
R654	317-0562-01	5.6 k	C	5	125 m	
R655	315-0152-02	1.5 k	C	5	250 m	
R656	321-0193-48	1 k	MF	1	125 m	
R657	311-1653-00	220	CP	20	50 m	
R658	317-0102-01	1 k	C	5	125 m	
R659	317-0241-01	240	C	5	125 m	
R661	315-0152-02	1.5 k	C	5	250 m	
R662	321-0193-48	1 k	MF	1	125 m	
R663	317-0562-01	5.6 k	C	5	125 m	
R665	317-0752-01	7.5 k	C	5	125 m	
R667	317-0220-01	22	C	5	125 m	
R668	317-0152-01	1.5 k	C	5	125 m	
R701 *	310-0679-00	900 k		1	250 m	
R702 *		111 k		1	250 m	
R703 *	310-0678-00	990 k		1	250 m	
R704 *		10.1 k		1	250 m	
R705		500 k		1	250 mm	
R706 *		1 M		1	250 m	
R707	310-0683-00	800 k		1	250 m	
R708		250 k		1	250 m	
R709		1 M		1	250 m	
R710	317-0150-01	15	C	5	125 m	612101
R711	315-0104-01	100 k	C	5	250 m	
R712	317-0101-01	100	C	5	125 m	
R713	317-0750-01	75	C	5	125 m	
R714	317-0152-01	1.5 k	C	5	125 m	
R715	317-0332-01	3.3 k	C	5	125 m	
R716	317-0113-01	11 k	C	5	125 m	609351
R717	311-1656-00	4.7 k	CP	20	50 m	
R718	317-0912-01	9.1 k	C	5	125 m	
R719	317-0102-01	1 k	C	5	125 m	
R721	311-1764-00	47 k	CMP	20	500 m	
R722	317-0203-01	20 k	C	5	125 m	
R723†	311-1672-00	47 k	CV	20	250 m	
R724	317-0913-01	91k	CF	5	125 m	612301
R725	317-0302-01	3 k	C	5	125 m	

† with switch

CIR REF	PART NUMBER	DESCRIPTION	Eff. Ser.No.
S1	260-1638-00	Time/Div	
S21	260-1429-00	Int/Ext Trig	
S22	260-1429-00	Polarity	
S23	260-1429-00	AC-TV	
S24	With R27	Auto	
S101	with R27	Auto	
S102	with R137	x5 gain	
S401	260-1429-00	Slide 125/250 V	
S402	260-1307-00	Slide Hi-Lo Line	
S403	with R308	Instrument On/Off	609451
S404	with R308	Instrument On/Off	
S405	with R306	Power On/Off	
S406	with R306	Power On/Off	
S601	260-1429-00	Slider AC-DC	
S602	260-1690-00	Volts/Div	
S631	with R723	On CH2	
S632	260-1401-00	Trig select	
S701	260-1429-00	AC-DC	
S702	260-1690-00	Volts/Div	
SK21	131-1654-00	BNC Ext. Trig.	
SK315	131-1268-00	2 mm Probe test Cal 0.3 V	
SK401	131-1735-00	External DC/Battery Check	
SK402	136-0389-00	Charging Check	610101
SK601	131-1654-00	B.N.C. 50Ω 73-10-01	
SK701	131-1654-00	B.N.C. 50Ω 73-10-01	
T401	120-0885-00	Power	
T411	120-0886-01	Inverter	

* thick film cermet resistor

CIR REF	PART NUMBER	VALUE	DESCRIPTION	TYPE	TOL %	RATING	Eff. Ser.No.
TH601	307-0288-00	1.3 kΩ	N.T.C. Type VH1038		20	0.5 W	
TH701	307-0288-00	1.3 kΩ	N.T.C. Type VH1038		20	0.5 W	

CIR REF	PART NUMBER	DESCRIPTION		TYPE	Eff. Ser.No.
TR21	151-0127-02	BSX20	Si	NPN	
TR22	151-0127-02	BSX20	Si	NPN	
TR23	151-0317-00	BC109C	Si	NPN	
TR24	151-0320-01	MPS6518	Si	PNP	
TR25	151-0320-01	MPS6518	Si	PNP	
TR26	151-0320-01	MPS6518	Si	PNP	
TR101	151-0320-01	MPS6518	Si	PNP	
TR102	151-0326-00	BC107	Si	NPN	
TR103	151-1076-00	WN537	Si		
TR104	151-0317-00	BC107	Si	NPN	612001
TR105	151-0326-00	BC107	Si	NPN	
TR106	151-0326-00	BC107	Si	NPN	
TR107	151-0242-00	2N3904	Si	NPN	
TR108	151-0320-01	MPS6518	Si	PNP	
TR109	151-0242-00	2N3904	Si	NPN	
TR111	151-0320-01	MPS6518	Si	PNP	
TR112	151-0242-00	2N3904	Si	NPN	
TR113	151-0242-00	2N3904	Si	NPN	
TR114	151-0320-01	MPS6518	Si	PNP	
TR301	151-0326-00	BC107	Si	NPN	
TR302	151-0525-03	FRB749	Si	NPN	
TR315	151-0320-00	MPS6518	Si	PNP	
TR316	151-0320-00	MPS6518	Si	PNP	
TR401	151-0320-00	MPS6518	Si	PNP	
TR402	151-0480-00	2SC1173 (R)	Si	NPN	

CIR REF	PART NUMBER	DESCRIPTION		TYPE	Eff. Ser.No.
TR411	151-0479-00	BDX36	Si	NPN	
TR412	151-0479-00	BDX36	Si	NPN	
TR601	151-1076-00	WN537A	Si		
TR602	151-0127-02	BSX20	Si	NPN	
TR603	151-0317-00	BC109C	Si	NPN	
TR604	151-0242-00	2N3904	Si	NPN	
TR631	151-0326-00	BC107	Si	NPN	
TR632	151-0326-00	BC107	Si	NPN	
TR633	151-0317-00	BC109C	Si	NPN	
TR651	151-0320-00	MPS6518	Si	PNP	
TR652	151-0242-00	2N3904	Si	NPN	
TR653	151-0242-00	2N3904	Si	NPN	
TR654	151-0320-00	MPS6518	Si	PNP	
TR701	151-1076-00	WN537A	Si		
TR702	151-0127-00	BSX20	Si	NPN	
TR703	151-0317-00	BC109C	Si	NPN	
TR704	151-0242-00	2N3904	Si	NPN	
V301	154-0706-00	CRT Type D10-193			

SUB ASSEMBLIES

For positions of the various sub assemblies see the exploded views, Section 6. Each main assembly comprises a number of smaller sub-assemblies, miscellaneous components and mechanical parts (see also mechanical parts list).

MAIN ASSEMBLY	SUB ASSEMBLY	PART NUMBER
R/H SIDE ASSEMBLY (Sweep and Calibrator)	PC172 wired	670-3529-01
	TIME/DIV switch	262-0978-00
L/H SIDE ASSEMBLY (Y Amplifier and chop/alternate bistable)	PC187 wired	670-3743-00
	VOLTS/DIV switch (CH1)	262-0977-00
	VOLTS/DIV switch (CH2)	262-0977-00
LOWER ASSEMBLY (Power and tube supplies)	PC173 wired	670-3530-00
CENTRE ASSEMBLY AND REAR PANEL (Tube assembly and line voltage selection	PC178 wired	670-3308-00

D32 MECHANICAL PARTS

FOR POSITIONS OF THE MECHANICAL PARTS SEE THE EXPLODED DRAWINGS WHICH FOLLOW

DRG.	PART NUMBER	DESCRIPTION	Effective Ser. No.
1	101-0026-00	Front Trim (LH)	
2	101-0025-00	Front Trim (RH)	
3	333-2050-00	Front Panel (TIME/DIV)	
4	333-2051-00	Front Panel (VOLTS/DIV)	
6	333-2207-00	Side Panel	
7	337-2123-02	Screen, Elec. (VOLT/DIV)	
8	333-1913-05	Front Panel (Control)	
9	337-2054-00	Screen, Cover	
10	343-0234-00	Cable Cleat	
11	313-0413-00	Graticule (Blue) Assembly	
		or	
	313-0414-00	Graticule (Amber) Assembly	
12	200-1657-01	Front Bezel (Side)	
13	101-0028-00	Front Bezel (Upper)	
14	200-1828-01	Front Bezel (Lower)	
16	407-1503-00	Bracket	
17	407-1502-00	Bracket	
18	381-0351-02	Bar	
19	441-1225-02	Centre Chassis	
20	343-0108-00	Cable Cleat	
21	333-1879-02	Rear Panel	
22	441-1384-00	Bottom Tray	
23	343-0512-00	Transformer Clamp	
24	376-0148-01	Flexible Coupling	
25	384-1381-00	Shaft Extension	
26	407-1821-00	Bracket fixing point	
27	361-0670-00	Spacer Pivot	
29	391-0143-01	Block (Voltage Identification)	
31	366-1654-00	Knob Assembly	
32	366-1657-01	Knob Assembly	
33	210-1247-00	Felt Washer	
34	358-0460-00	Bush	
36	366-1656-01	Knob Assembly	
38	334-2227-01	Rear Label	
39	366-1414-15	Knob-Push Button-Assembly	
40	376-0136-00	Coupling	
41	376-0132-00	Switch Extension Coupling	
42	384-1141-08	Extension Rod	
44	220-0727-00	Type 'U' Nut	
46	200-1863-01	Cover	
47	134-0154-00	Power Plug	
48	200-1675-01	Transformer Cover	
49	334-2552-03	Name Plate (Serial No.)	
51	343-0500-01	Clamp (C402)	
52	334-2633-00	Label (Fuse Identification)	
53	352-0447-00	Battery Holder (see Mechanical Assembly)	
54	101-0027-02	Handle Trim (LH)	
55	101-0027-03	Handle Trim (RH)	
56	166 0511-00	Insulating Sleeve	611675
58	437-0186-00	Cover Cabinet	
59	367-0208-02	Handle (LH)	
60	367-0208-03	Handle (RH)	
62	214-2286-01	Index Ring (RH)	
63	214-2286-02	Index Ring (LH)	
64	105-0680-00	Handle Catch	
65	214-2287-00	Handle Spring	
66	200-1830-01	Handle Cover	
67	367-0207-01	Handle Grip	
68	210-1235-00	Handle, Washer Assembly	
69	200-2126-00	Fuse cover	612201
71	337-2008-00	Gun Shield (CRT)	
72	220-0527-00	Nut Ring	
73	378-0836-00	Screen	
74	348-0167-01	Foot	
75	200-0882-01	Cap	
77	200-1725-01	Warning Cover	
78	384-0941-00	Extension Rod	
79	437-0171-01	Front Cover Protection	
80	361-0275-00	Spacer Bush	
81	407-1500-00	Bracket Heatsink	
82	131-1259-00	Earthing Contact	
83	210-0297-00	Solder Tag 6BA	
84	343-0207-00	Cable Cleat	
86	213-0460-00	Screw 8BA CH HD x ¼"	
87	213-0694-00	Screw 8BA CH HD x 5/16"	
88	213-0454-00	Screw 8BA CSK HD x ¼"	
89	213-0720-00	Screw 8BA R/CSK HD x ⅛	
90	213-0699-00	Screw 8BA R/CSK HD x 3/8	
91	213-0392-00	Screw 6BA PAN HD x 3/16	
92	213-0393-00	Screw 6BA PAN HD x ¼"	
94	213-0406-00	Screw 6BA PAN HD x 3/8"	
95	213-0395-00	Screw 6BA PAN HD x 1	
96	21300321-00	Screw 6BA CH HD x ¼"	
97	213-0391-00	Screw 6BA CSK HD x ¼"	
98	213-0400-00	Screw 6BA CSK HD x 3/8"	
99	213-0730-00	Screw 6BA CH HD x ½"	
100	213-0403-00	Screw 4BA CSK HD x ½"	
101	213-0515-00	Screw 2BA PAN HD x ½"	
103	213-0248-00	Screw Set M3 x 3mm	
105	213-0354-00	Screw S/T No 2 Type B PAN HD x ¼"	
106	213-0727-00	Screw S/T No 4 Type B PAN HD x 3/8"	
111	210-1213-00	Washer 8BA Small	
112	210-1211-00	Washer 8BA Large	
113	210-1214-00	Washer 8BA Shakeproof	
114	210-1159-00	Washer 6BA SRBP	
115	210-1207-00	Washer 6BA Large	
116	210-1209-00	Washer 6BA Small	
117	210-1210-00	Washer 6BA Shakeproof	
	210 1079-00	Washer, Lock 3/8"i.d. ½" o.d	611701
120	210-1203-00	Washer 2BA Shakeproof	
121	220-0719-00	Nut 8BA (HALF)	
122	220-0718-00	Nut 8BA (FULL)	
123	220-0717-00	Nut 6BA (HALF)	
124	220-0716-00	Nut 6BA (FULL)	
128	220-0693-00	Nut (Angle)	
129	213-0280-00	Screw 6BA Nylon	
131	220-0720-00	Nut 6BA Nylon	

SECTION 6
CIRCUIT DIAGRAMS

To minimize the risk of misinterpretation of component values on circuit diagrams, the decimal point has been replaced by the multiplier or sub-multiplier of the basic unit. For instance, 2.2 megohms is shown as 2M2 and 1.8 picofarads is shown as 1p8.

To aid the reader further, in addition to the block Circuit Reference Table in Section 6, to locate a component in the circuit diagrams, a table is provided at the top of each circuit diagram, in which the circuit reference will appear, where practicable, directly above the component being sought.

Each figure shows the appropriate Printed Circuit Board for the particular circuitry but the table below gives a complete quick reference guide to that information.

FIGURE	CIRCUIT(s)	P.C. BOARD
1	Channel 1 Input Stage	187
2	Channel 2 Input Stage	187
3	Y Output and Chop – Alternate Bistable	187
4	Trigger	172
5	Sweep Generator, Unblanking and X Amp	172
6	Calibrator and CRT	173
7	Battery Charger and Power Supply	173 178

| | | |

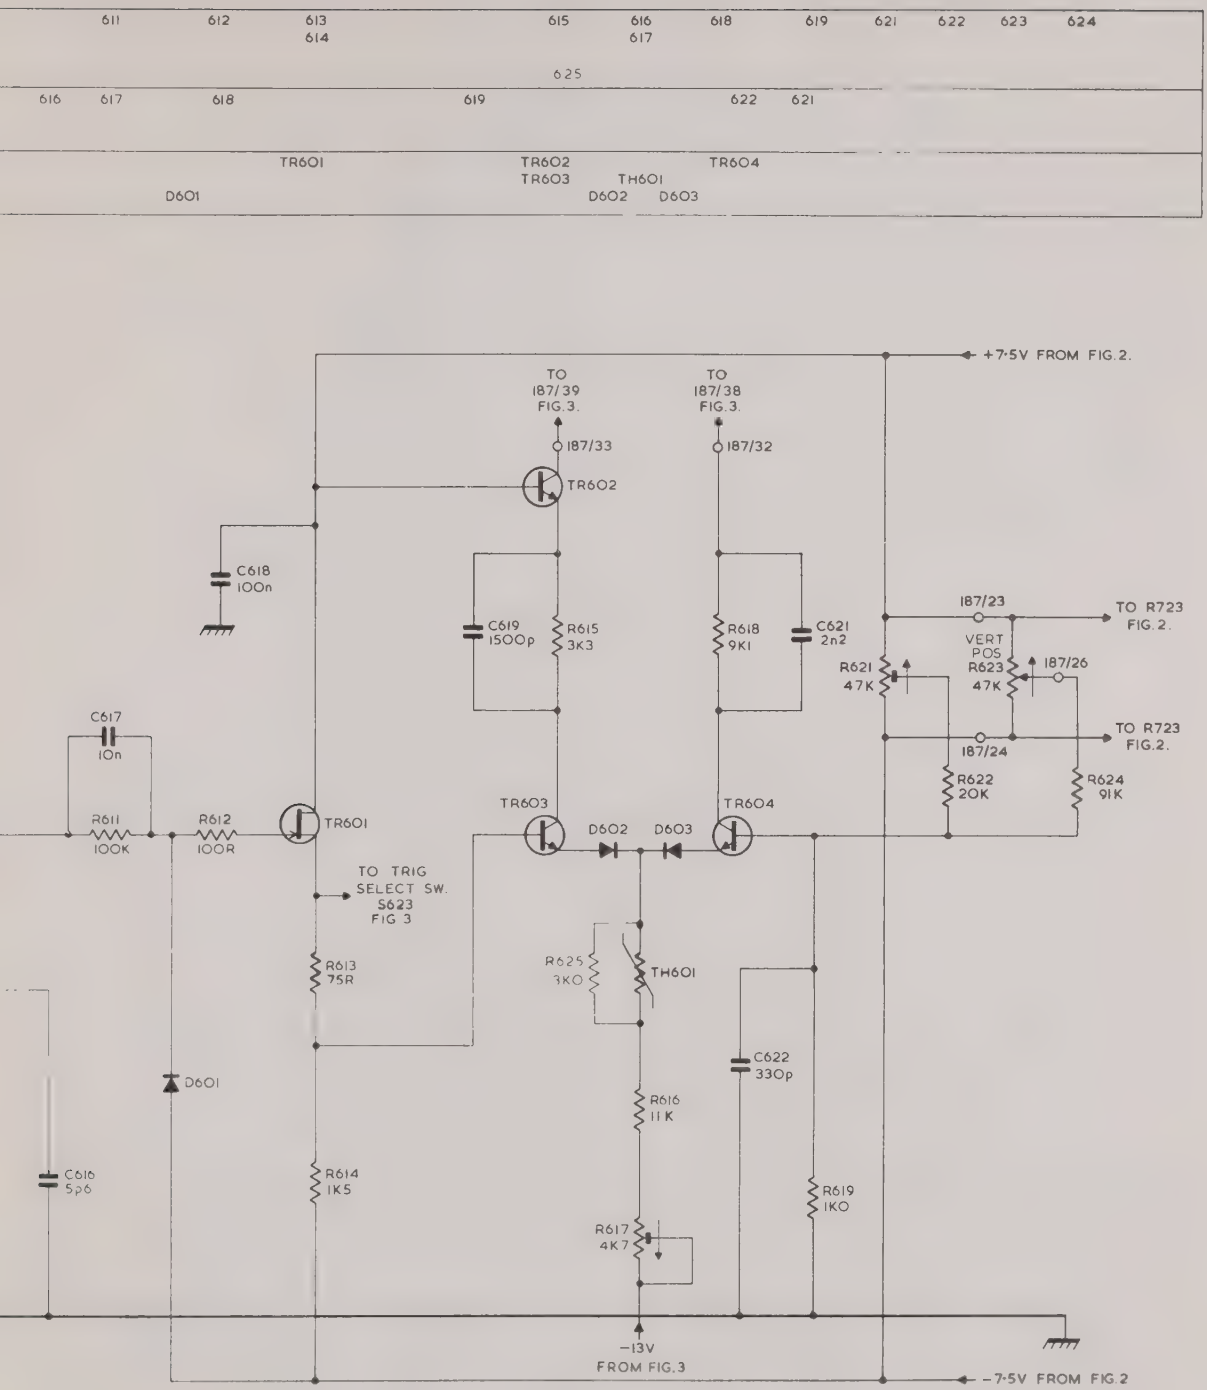

CHANNEL I INPUT STAGE D32
PC 187 FIG.1.

RESISTORS		701 702	710	703 704			705 706	707 708	709
CAPACITORS	702 703	704 701	705 707 708	706		709 711	712	713 714 715	
MISC.					S702				
SK701	701								

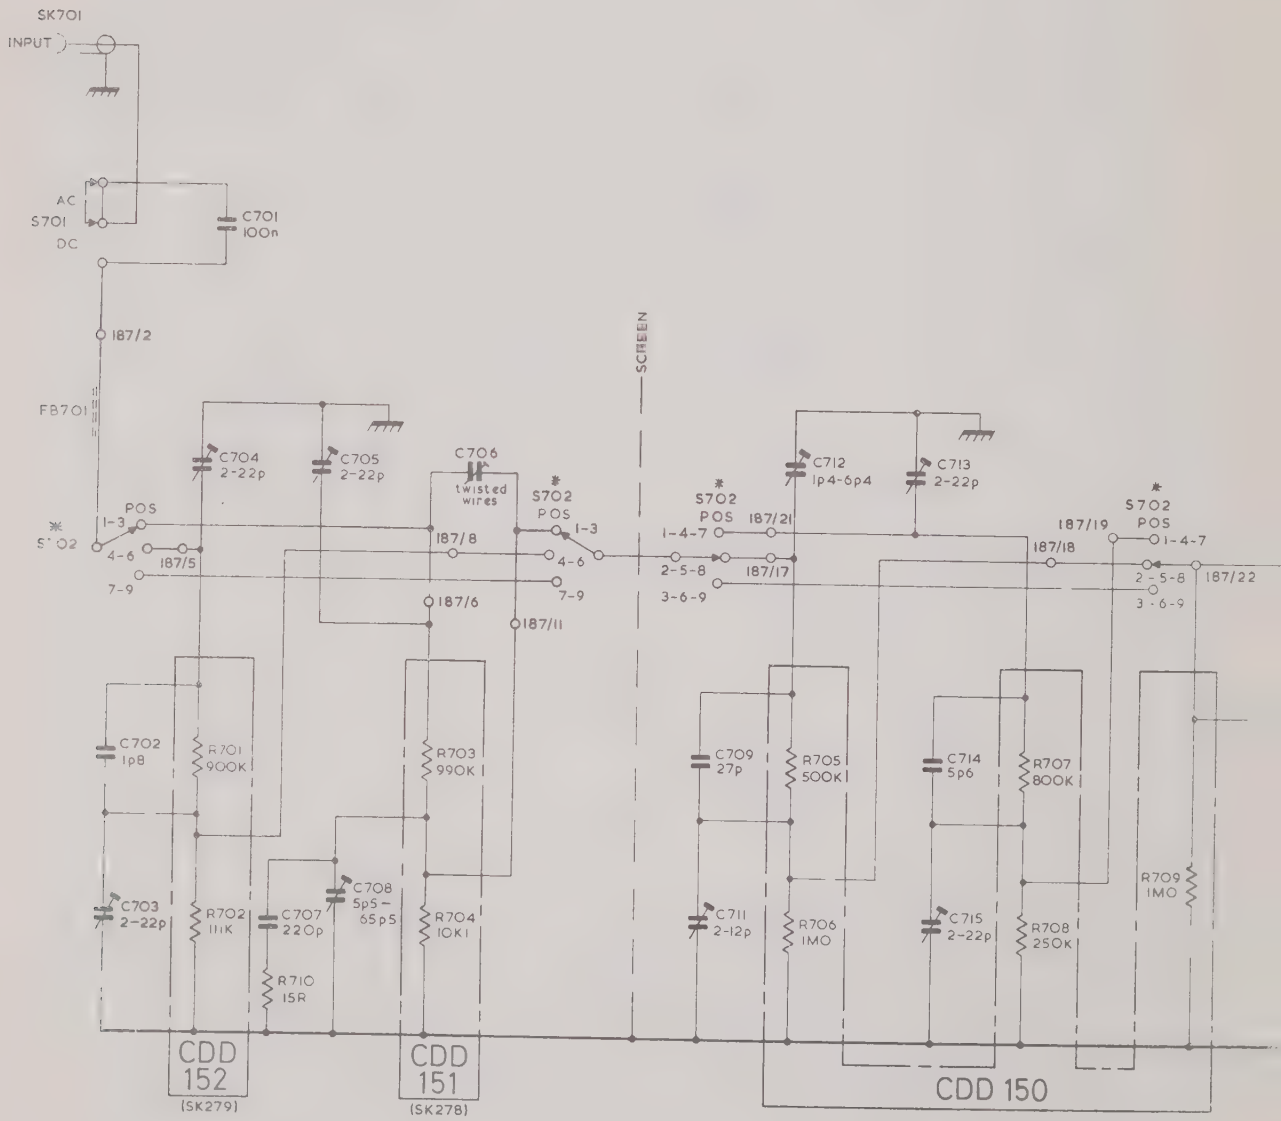

NOTES

1. 187/1 DENOTES P.C. BOARD/EYELET OR TERMINAL No CONNECTOR.
2. ✱ DENOTES COMPONENTS NOT MOUNTED ON P.C. BOARD

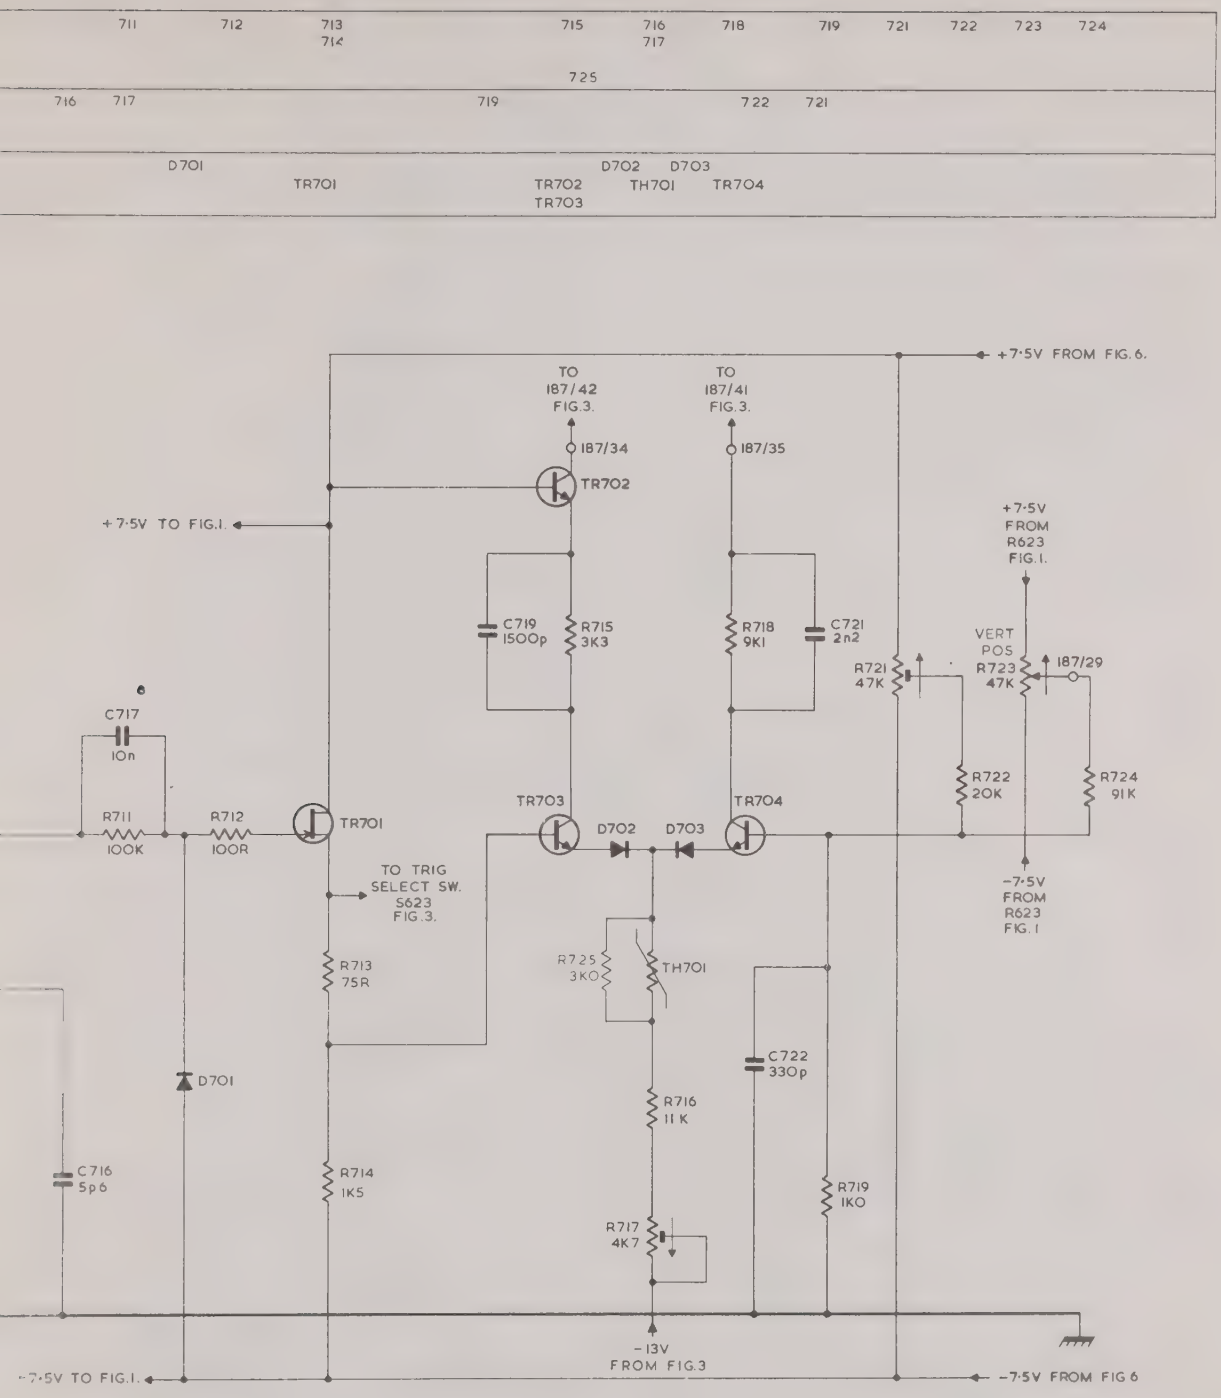

CHANNEL II INPUT STAGE D32

PC187 FIG. 2

| | | |

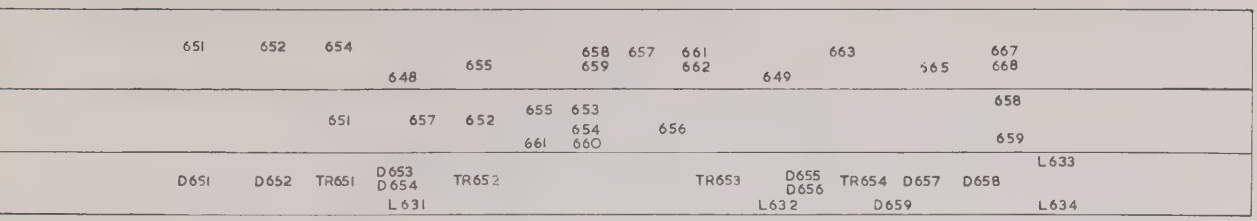

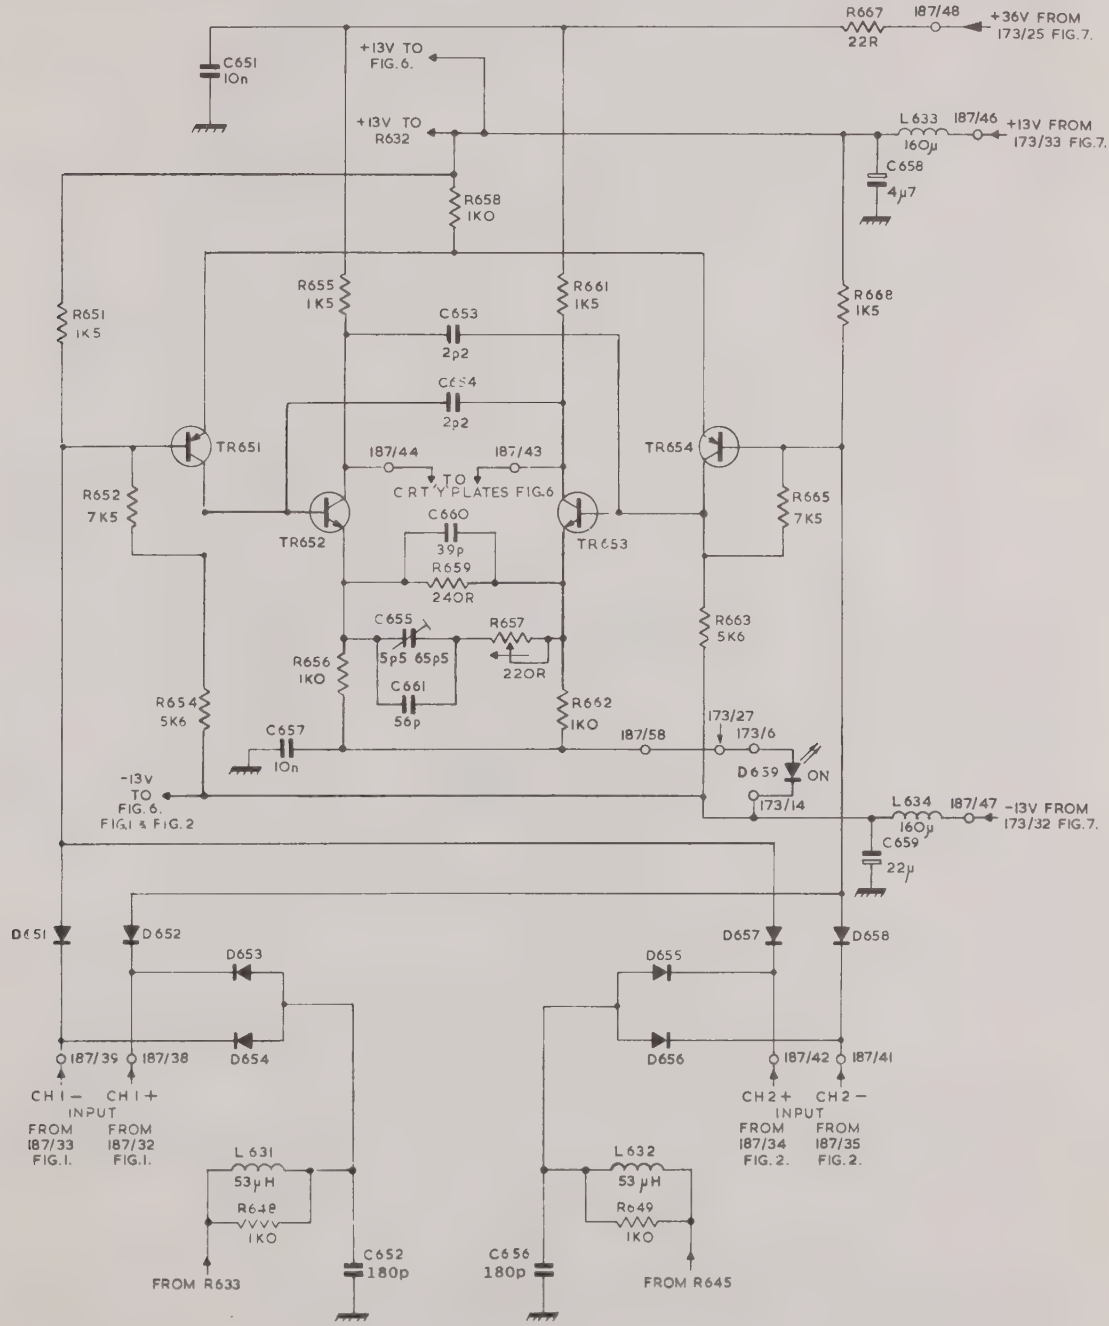

NOTES.

1. * DENOTES COMPONENTS NOT MOUNTED ON PC BOARD
2. DENOTES PC BOARD/EYELET OR TERMINAL No CONNECTION

| | | |

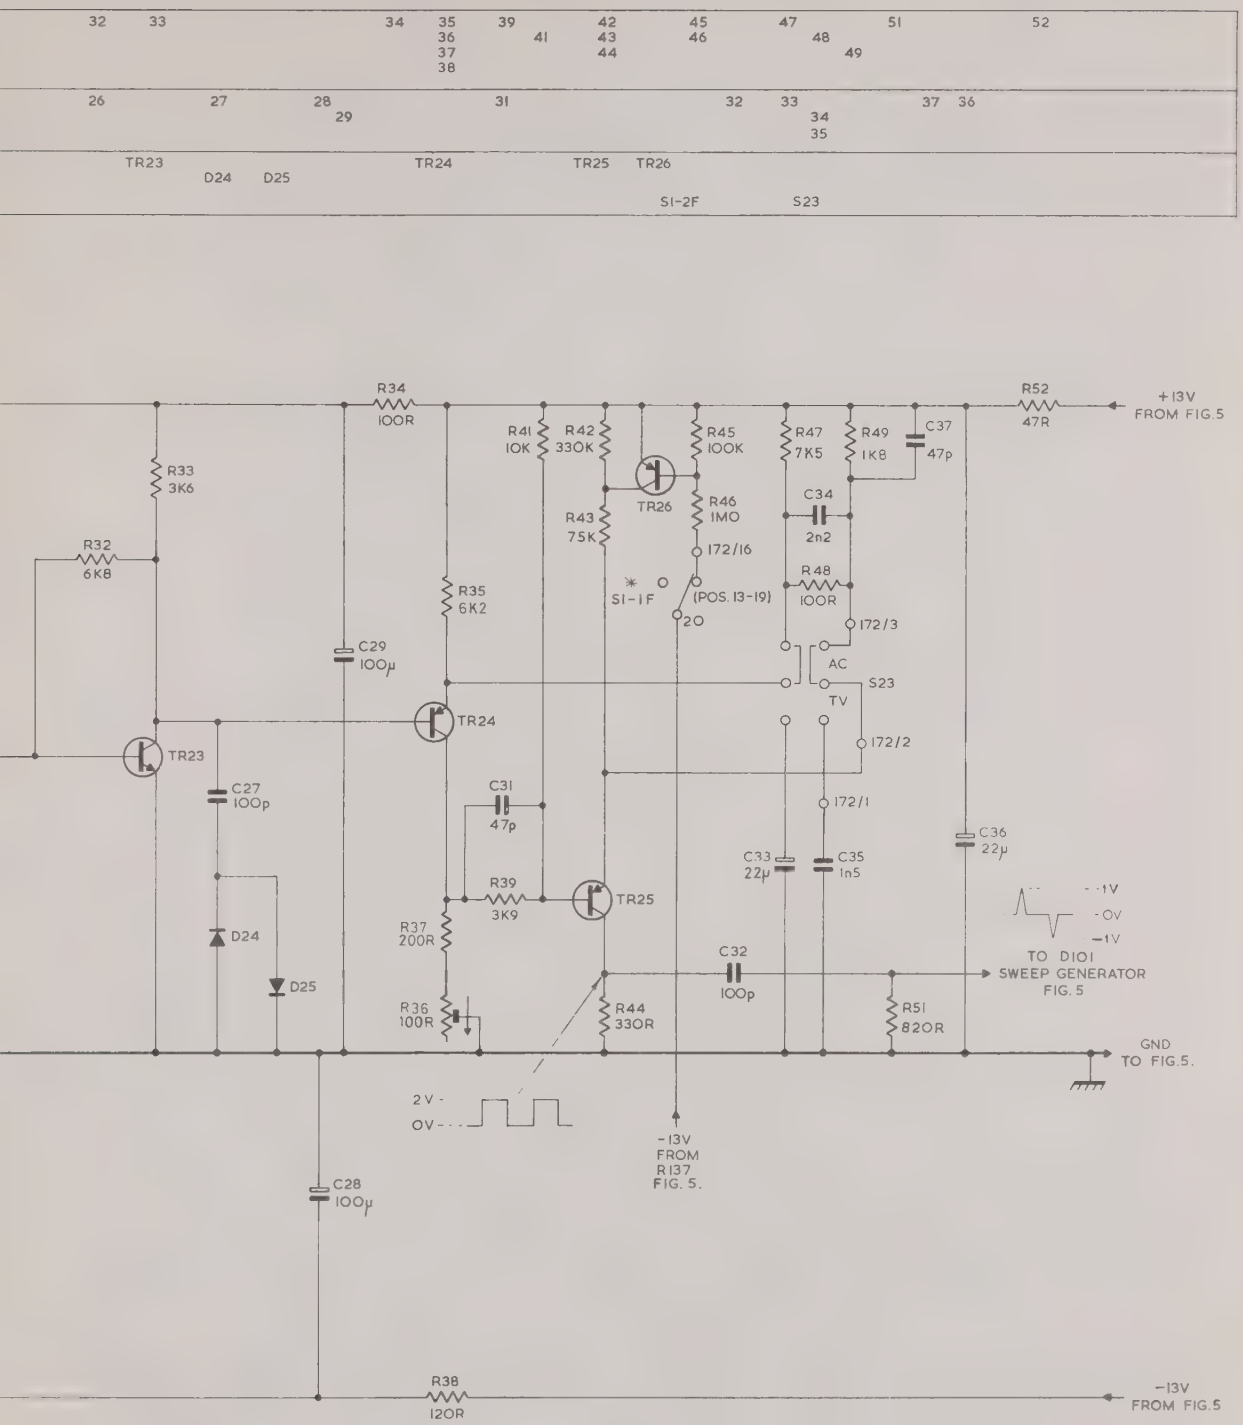

D32 TRIGGER CIRCUIT – P.C.172.

FIG. 4

| | | |

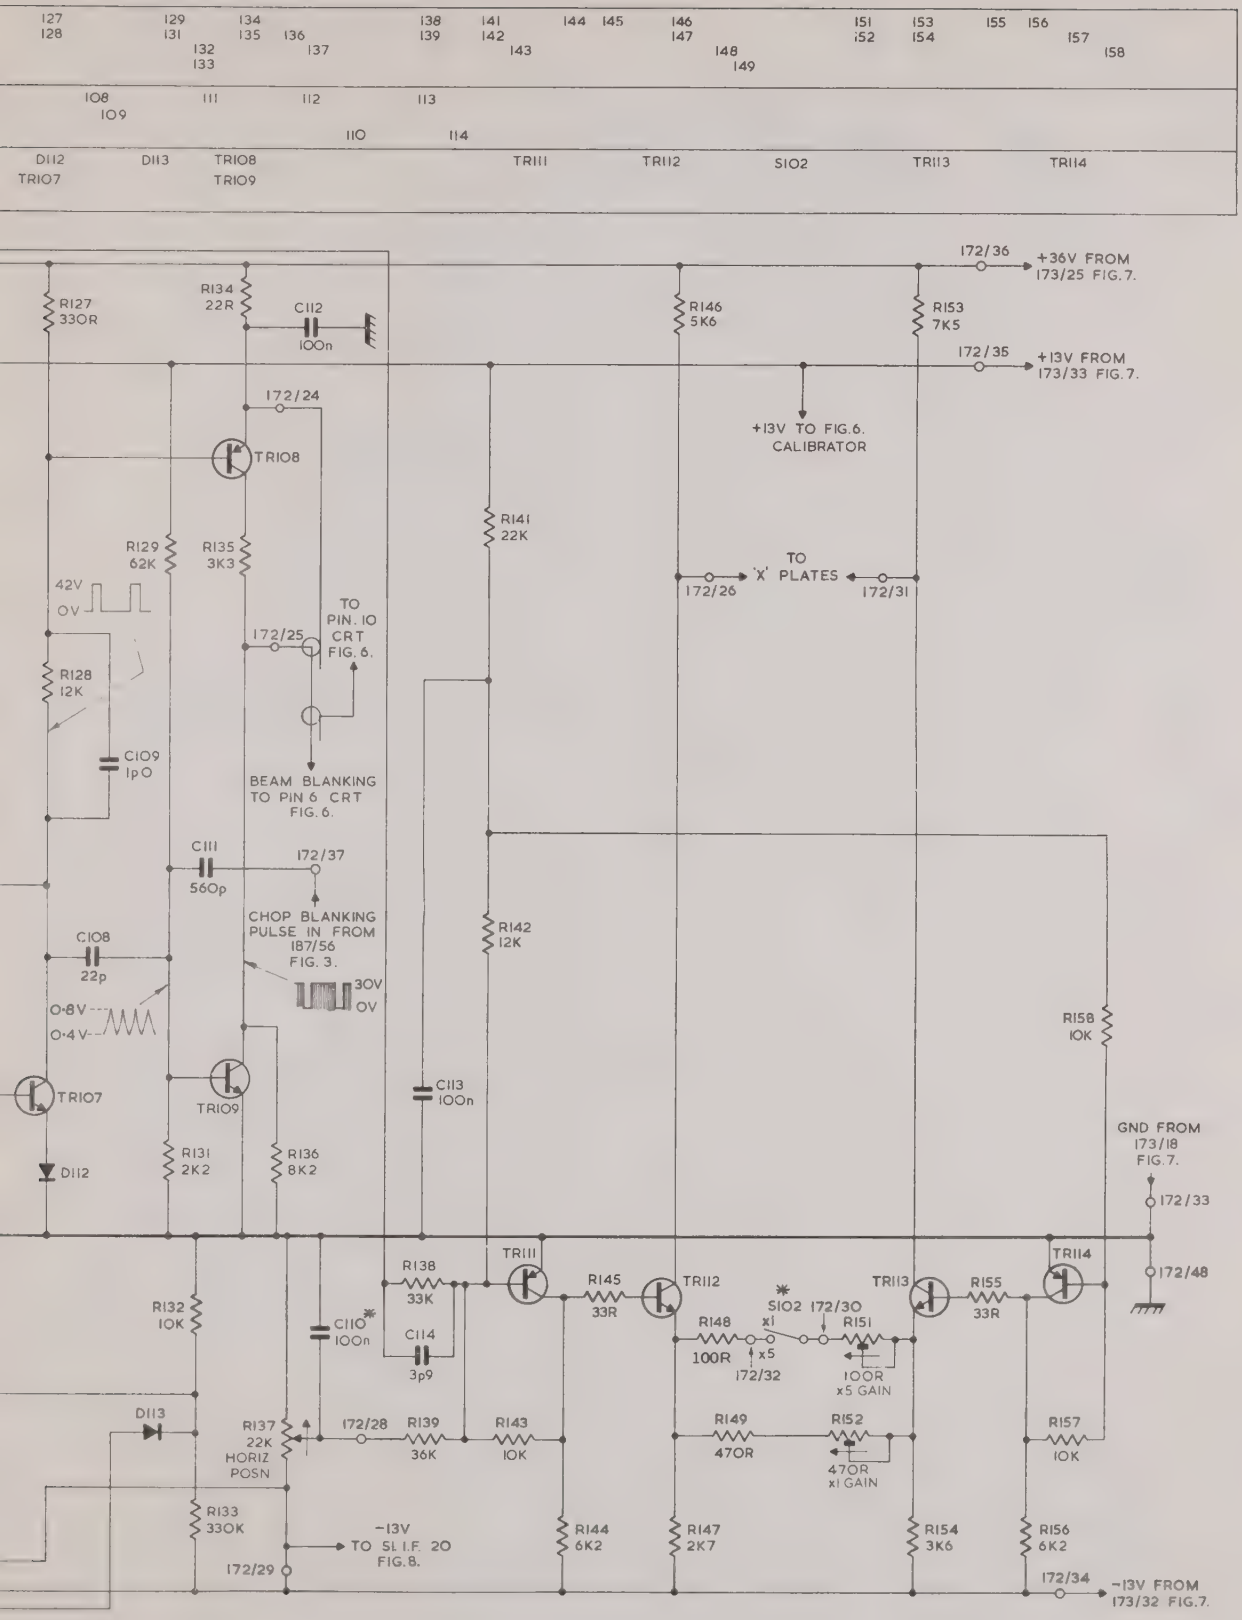

D32 SWEEP GENERATOR. UNBLANKING & 'X' AMP — P.C.172

FIG. 5.

5R
11/77

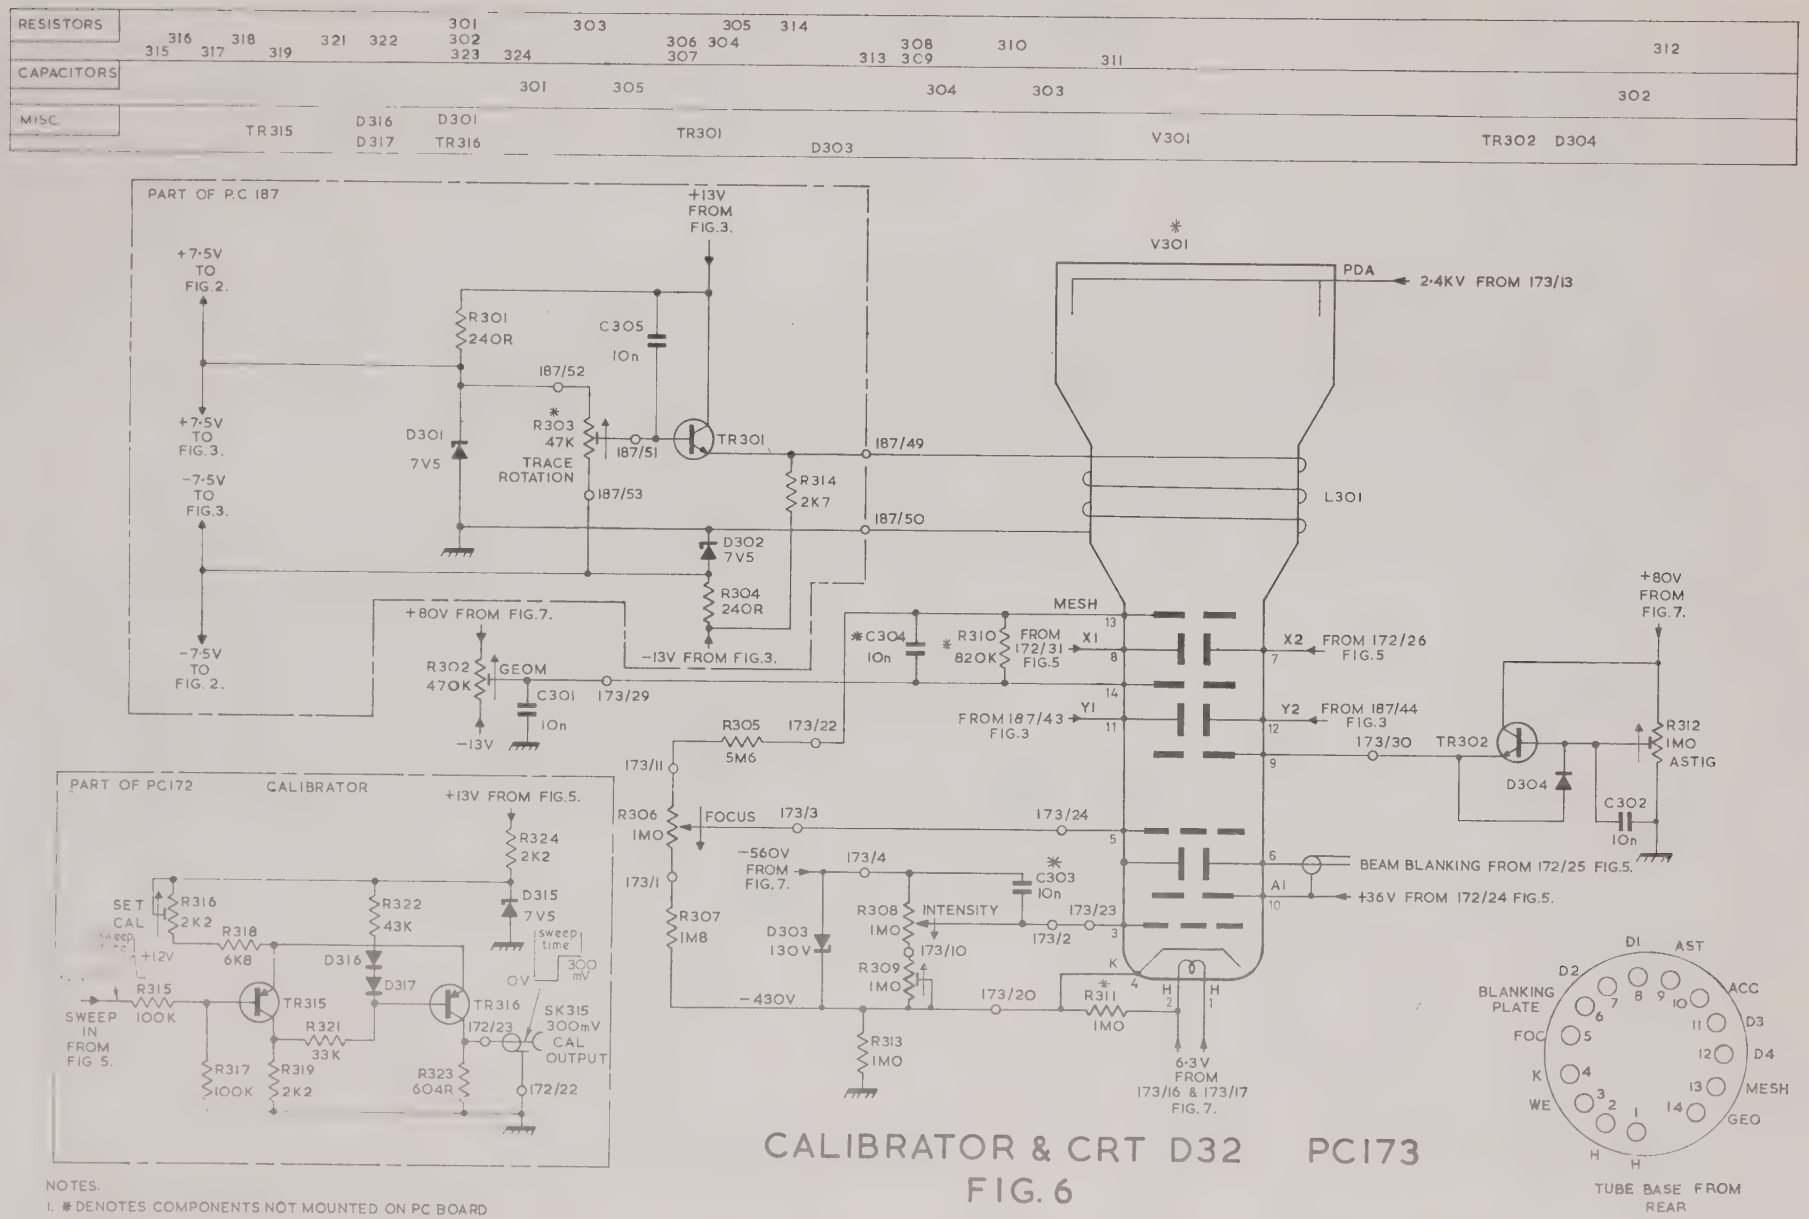

NOTES.
1. * DENOTES COMPONENTS NOT MOUNTED ON PC BOARD
2 173/29 DENOTES PC BOARD/EYELET OR TERMINAL No CONNECTION

CALIBRATOR & CRT D32 PC173
FIG. 6

| | | |

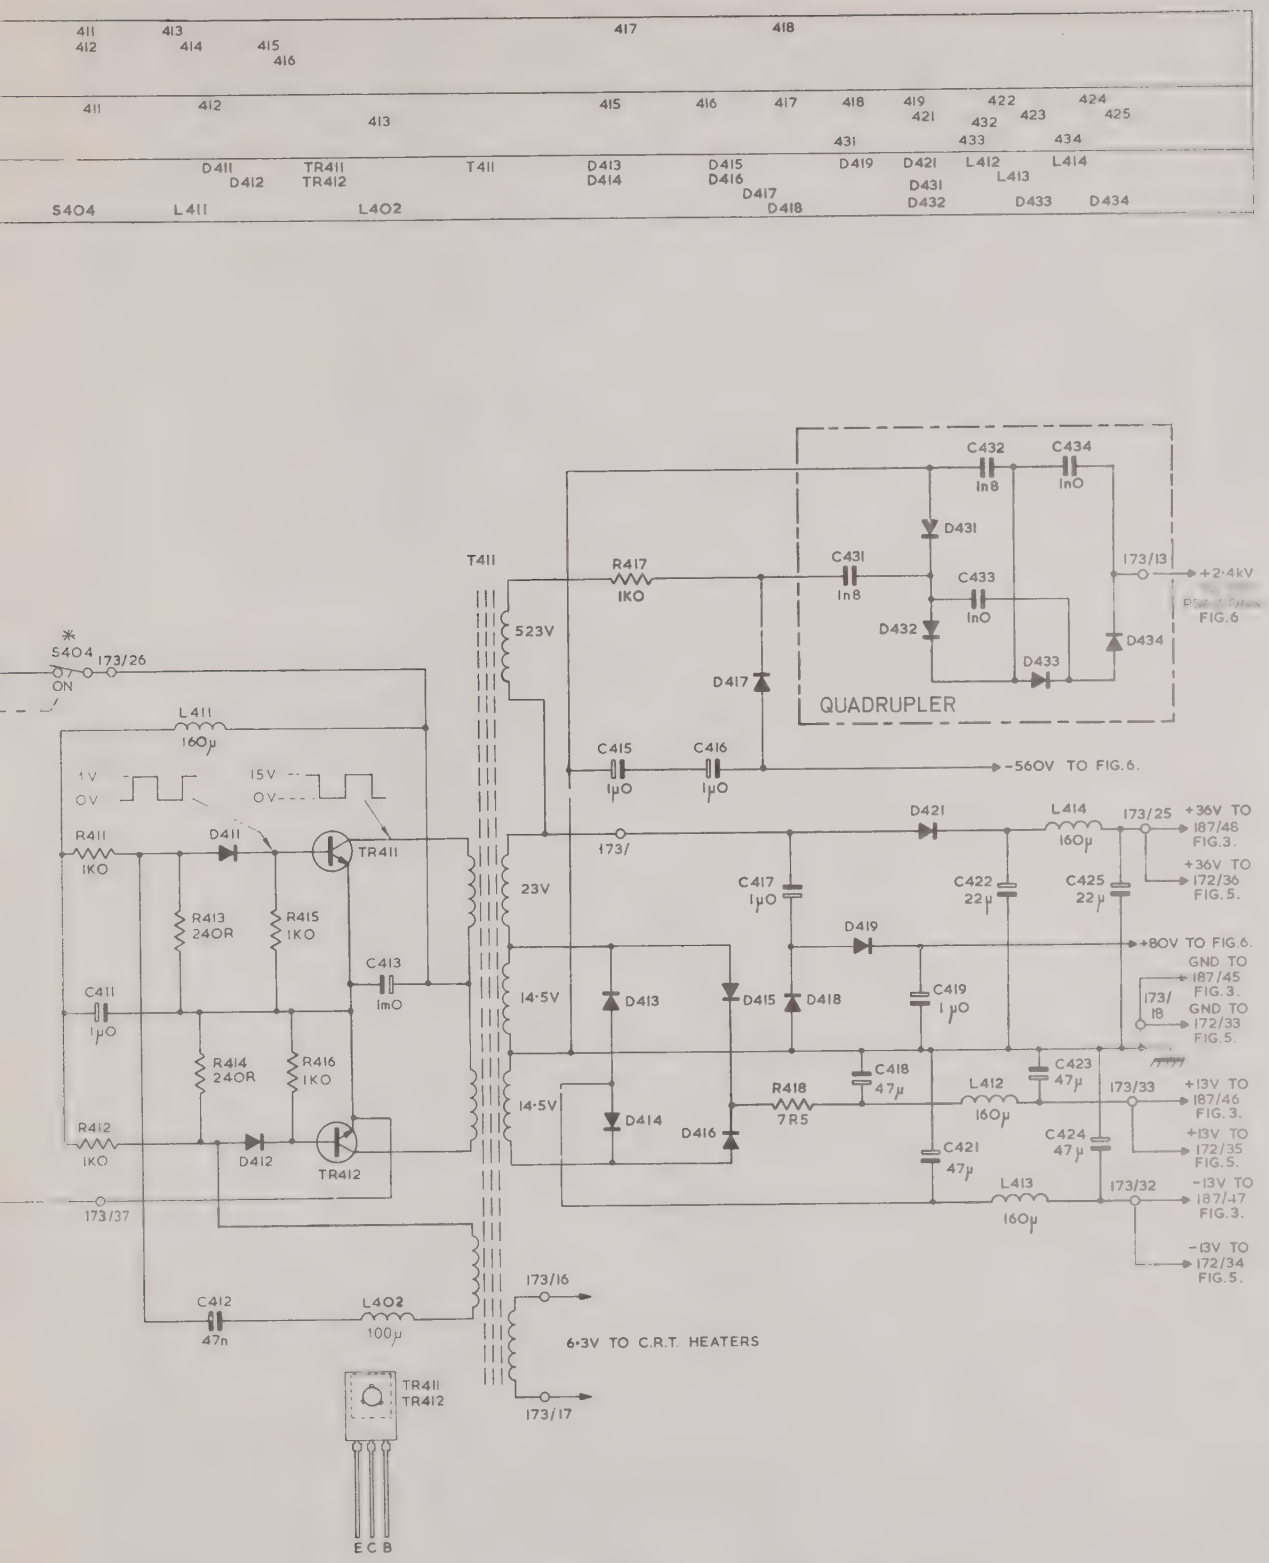

POWER SUPPLY PC173 D32

FIG. 7

| | | |

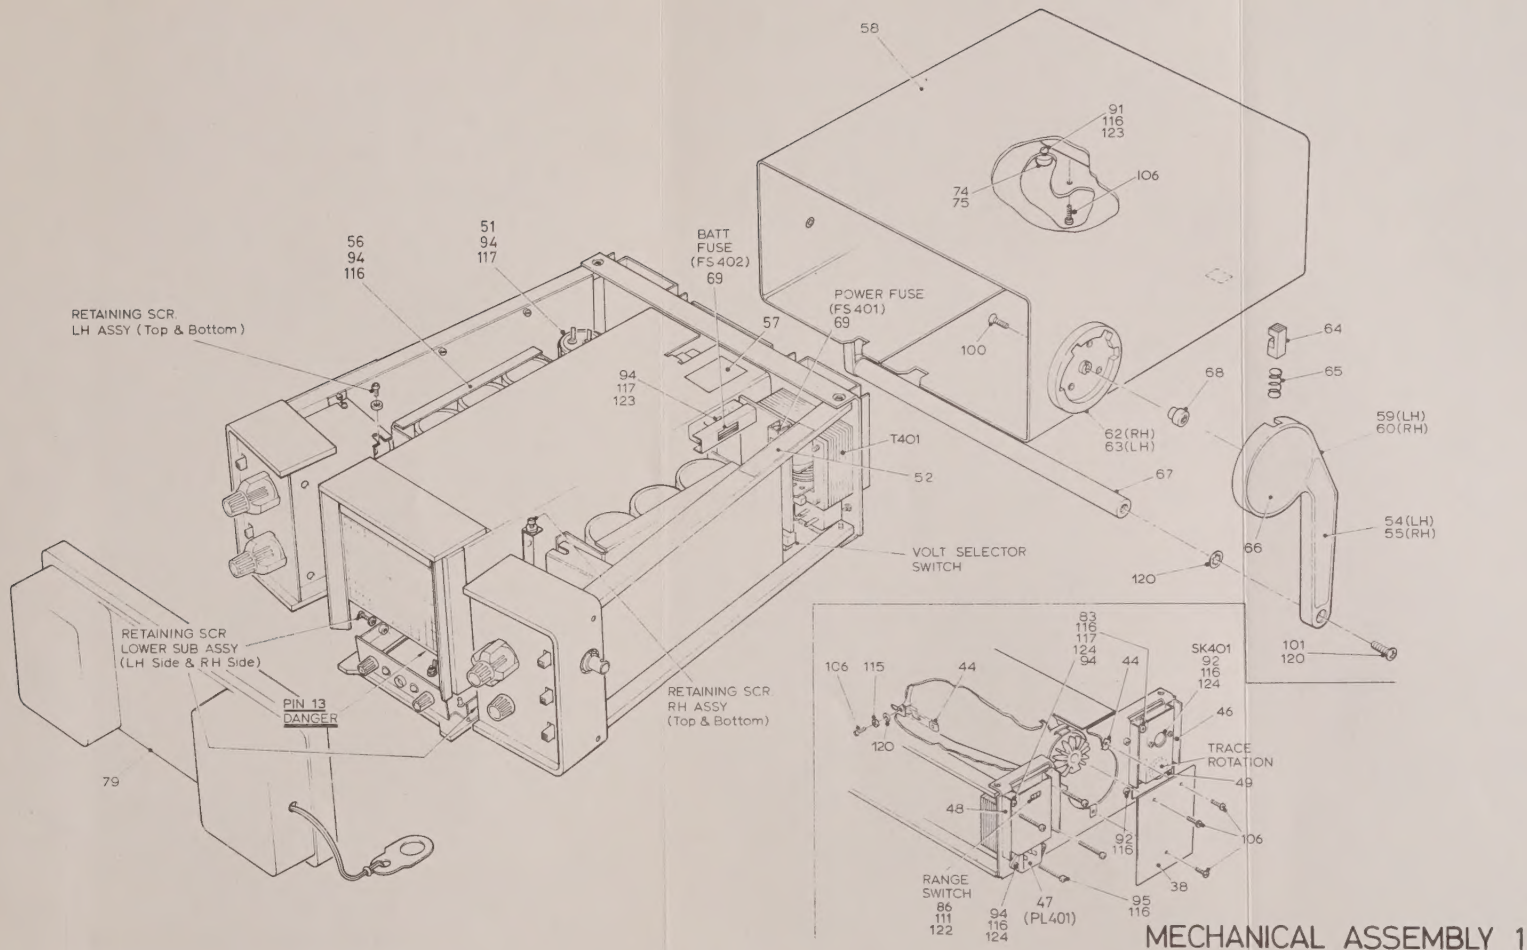

MECHANICAL ASSEMBLY 1
D32

11.2.77

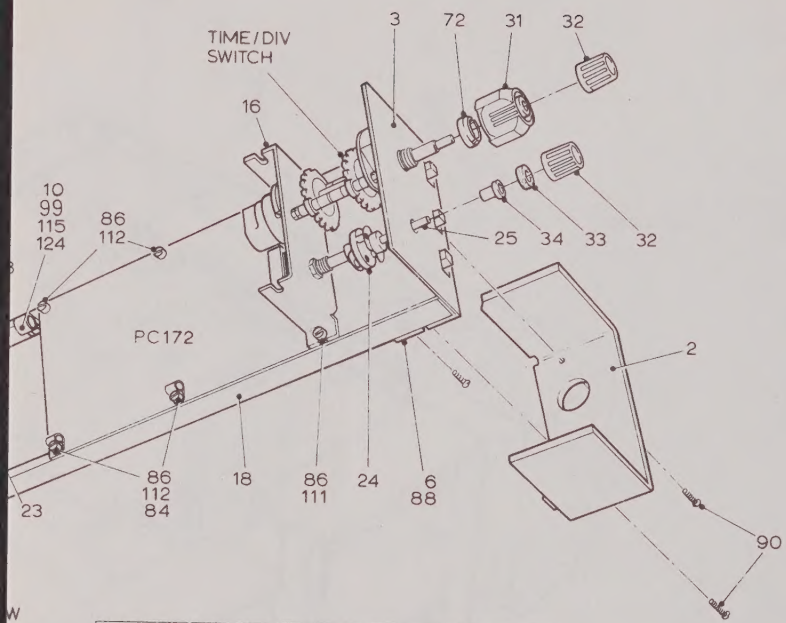

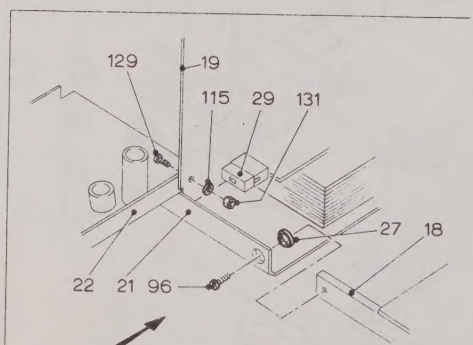

VIEW A (SHOWING TRAY, TYPICAL HINGE FOR VOLT/DIV. & TIME/DIV. ASSY

MECHANICAL ASSEMBLY 2
D32

www.manualsplus.com
1004108